


Air and Emissions Fibers

Shipment: 394 **Matrix:** Air and Emissions
Analyte: Fibers
Sample: 7499
Technology: PCM
Prep Method:
Target: 244.08 Fibers per mm2
Limits: 46.3 to 496 Fibers per mm2
Basis: Robust Statistics (Normal Distribution)
Robust Mean: 274.4 Fibers per mm2
Std Dev: 81.8669 Fibers per mm2
Median: 275.1 Fibers per mm2

Totals for Matrix/Analyte/Technology:

Labs: Pass: 84 **Fail:** 1 **Total:** 85

Totals for Matrix/Analyte: **Labs:** Pass: 84 **Fail:** 1 **Total:** 85

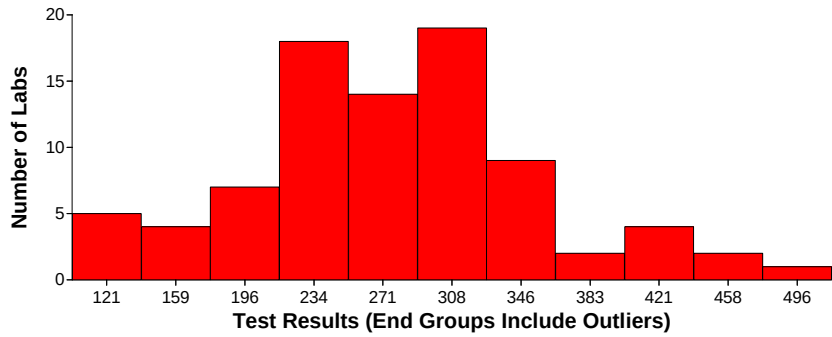


Air and Emissions Fibers

Shipment: 394 **Matrix:** Air and Emissions
Analyte: Fibers
Sample: 8272
Technology: PCM
Prep Method:
Target: 844.7 Fibers per mm2
Limits: 139 to 1420 Fibers per mm2
Basis: Robust Statistics (Normal Distribution)
Robust Mean: 777.2 Fibers per mm2
Std Dev: 230.08 Fibers per mm2
Median: 799.36 Fibers per mm2

Totals for Matrix/Analyte/Technology:

Labs: Pass: 84 **Fail:** 1 **Total:** 85

Totals for Matrix/Analyte: **Labs:** Pass: 84 **Fail:** 1 **Total:** 85

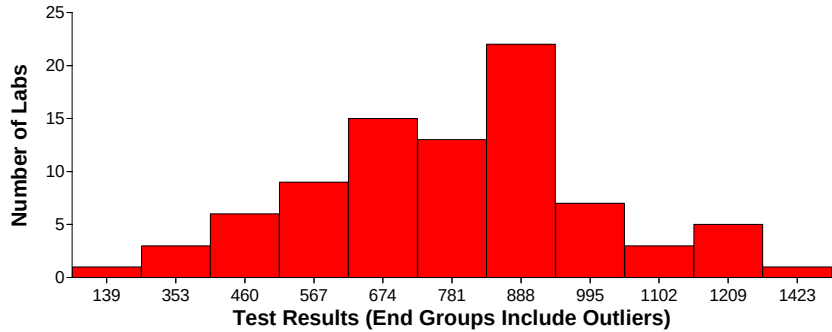


Air and Emissions Fibers

Shipment: 394 **Matrix:** Air and Emissions
Analyte: Fibers
Sample: 9433
Technology: PCM
Prep Method:
Target: 92.4 Fibers per mm2
Limits: 10 to 148 Fibers per mm2
Basis: Manual Limits
Robust Mean: 74.1 Fibers per mm2
Std Dev: 26.8738 Fibers per mm2
Median: 73 Fibers per mm2

Totals for Matrix/Analyte/Technology:

Labs: Pass: 83 **Fail:** 2 **Total:** 85

Totals for Matrix/Analyte: **Labs:** Pass: 83 **Fail:** 2 **Total:** 85

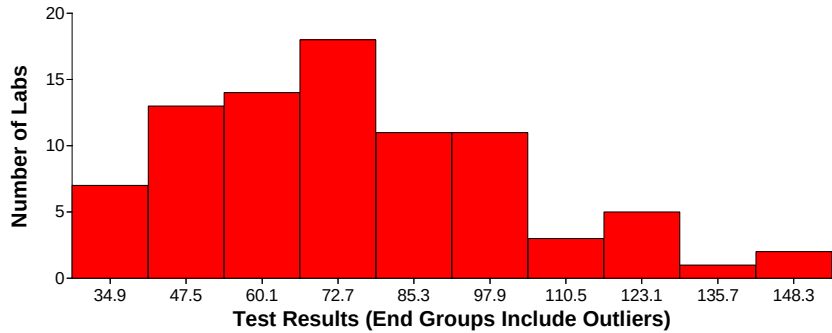


Air and Emissions Fibers

Shipment: 394 **Matrix:** Air and Emissions
Analyte: Fibers
Sample: 9855
Technology: PCM
Prep Method:
Target: 653 Fibers per mm2
Limits: 128 to 1090 Fibers per mm2
Basis: Robust Statistics (Normal Distribution)
Robust Mean: 616 Fibers per mm2
Std Dev: 198.6012 Fibers per mm2
Median: 612 Fibers per mm2

Totals for Matrix/Analyte/Technology:

Labs: Pass: 82 **Fail:** 3 **Total:** 85

Totals for Matrix/Analyte: **Labs:** Pass: 82 **Fail:** 3 **Total:** 85

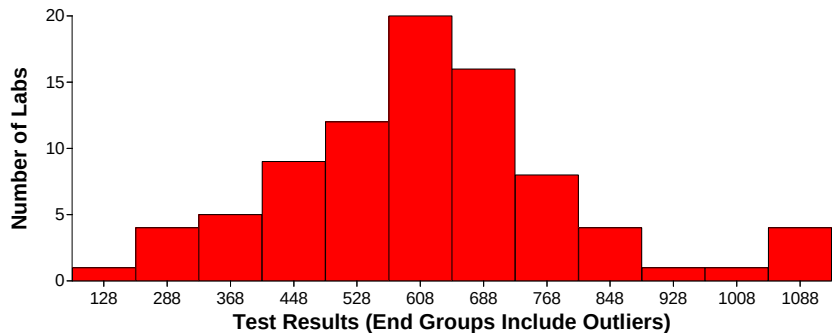

Solid and Hazardous Waste Asbestos in Friable Material


Solid and Hazardous Waste Asbestos in Friable Material

Shipment: 394 Matrix: Solid and Hazardous Waste
Analyte: Asbestos in Friable Material
Sample: 4699
Technology: PLM
Prep Method:
Target: 9 %
Limits: 1 to 15 %
Basis: Swa scoring
Robust Mean: 7 %
Std Dev: 3.9896 %
Median: 6.1 %

Totals for Matrix/Analyte/Technology:

Labs: Pass: 63 Fail: 8 Total: 71

Totals for Matrix/Analyte: Labs: Pass: 63 Fail: 8 Total: 71

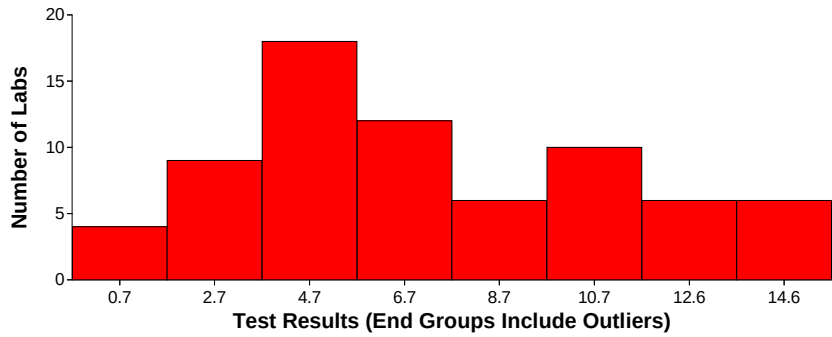


Solid and Hazardous Waste Asbestos in Friable Material

Shipment: 394 Matrix: Solid and Hazardous Waste
Analyte: Asbestos in Friable Material
Sample: 6523
Technology: PLM
Prep Method:
Target: 2.6 %
Limits: 1 to 12 %
Basis: Swa scoring
Robust Mean: 6.2 %
Std Dev: 3.1048 %
Median: 5.75 %

Totals for Matrix/Analyte/Technology:

Labs: Pass: 64 Fail: 7 Total: 71

Totals for Matrix/Analyte: Labs: Pass: 64 Fail: 7 Total: 71

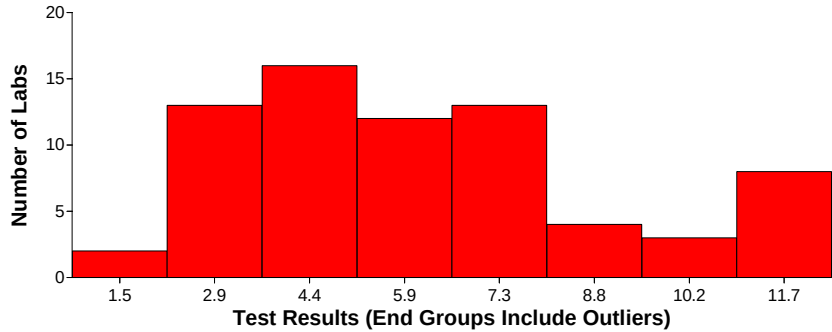


Solid and Hazardous Waste Asbestos in Friable Material

Shipment: 394 Matrix: Solid and Hazardous Waste
Analyte: Asbestos in Friable Material
Sample: 8364
Technology: PLM
Prep Method:
Target: 3 %
Limits: 0.2 to 3.3 %
Basis: Swa scoring
Robust Mean: 1.3 %
Std Dev: 0.6627 %
Median: 1.275 %

Totals for Matrix/Analyte/Technology:

Labs: Pass: 57 Fail: 14 Total: 71

Totals for Matrix/Analyte: Labs: Pass: 57 Fail: 14 Total: 71

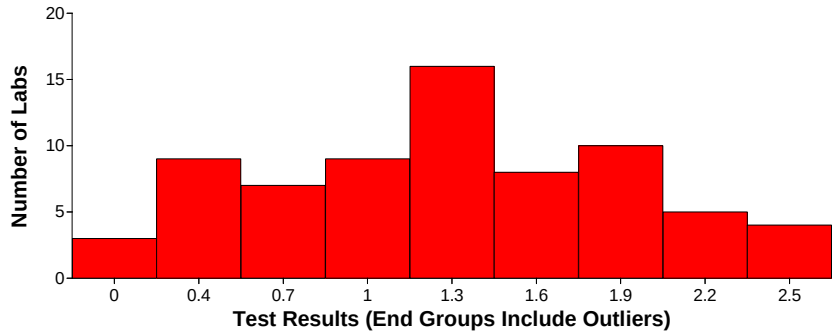

Solid and Hazardous Waste Asbestos in Friable Material

Shipment: 394 Matrix: Solid and Hazardous Waste
Analyte: Asbestos in Friable Material
Sample: 9745
Technology: PLM
Prep Method:
Target: 69.6 %
Limits: 18 to 91 %
Basis: Swa scoring
Robust Mean: 53.8 %
Std Dev: 17.5735 %
Median: 53.3 %

Totals for Matrix/Analyte/Technology:

Labs: Pass: 71 Fail: 0 Total: 71

Totals for Matrix/Analyte: Labs: Pass: 71 Fail: 0 Total: 71

