


Potable Water 1,1,1,2-Tetrachloroethane

Shipment: 407 Matrix: Potable Water
Analyte: 1,1,1,2-Tetrachloroethane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 17.8 ug/L
Limits: 14.2 to 21.4 ug/L
Basis: Fixed Percent (2)
Robust Mean: 17.9 ug/L
Std Dev: 3.6538 ug/L
Median: 17.9 ug/L

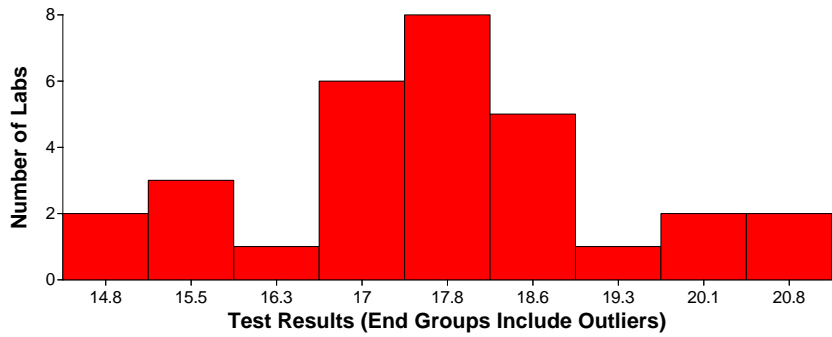

Totals for Matrix/Analyte/Technology:

Labs: Pass: 27 Fail: 3 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 28 Fail: 3 Total: 31

Potable Water 1,1,1,2-Tetrachloroethane

Shipment: 407 Matrix: Potable Water
Analyte: 1,1,1,2-Tetrachloroethane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 17.8 ug/L
Limits: 14.2 to 21.4 ug/L
Basis: Fixed Percent (2)
Robust Mean: 16.9 ug/L
Std Dev: 0 ug/L
Median: 16.9 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 28 Fail: 3 Total: 31

Potable Water 1,1,1-Trichloroethane

Shipment: 407 Matrix: Potable Water
Analyte: 1,1,1-Trichloroethane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 2.91 ug/L
Limits: 1.75 to 4.07 ug/L
Basis: Fixed Percent (2)
Robust Mean: 3 ug/L
Std Dev: 0.6606 ug/L
Median: 3 ug/L

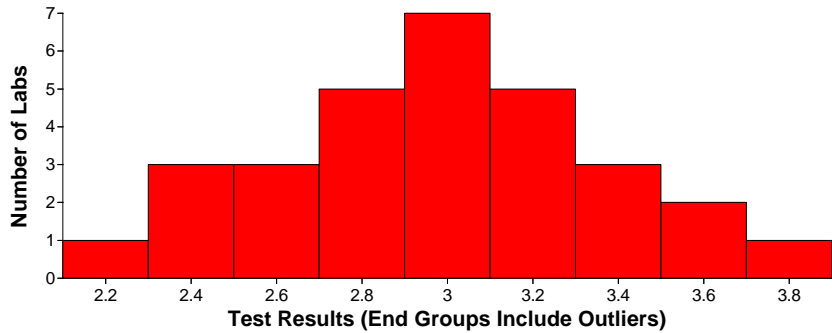

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water 1,1,1-Trichloroethane

Shipment: 407 Matrix: Potable Water
Analyte: 1,1,1-Trichloroethane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 2.91 ug/L
Limits: 1.75 to 4.07 ug/L
Basis: Fixed Percent (2)
Robust Mean: 3.5 ug/L
Std Dev: 0 ug/L
Median: 3.52 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water 1,1,2,2-Tetrachloroethane

Potable Water 1,1,2,2-Tetrachloroethane

Shipment: 407 Matrix: Potable Water
Analyte: 1,1,2,2-Tetrachloroethane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 10.3 ug/L
Limits: 8.24 to 12.4 ug/L
Basis: Fixed Percent (2)
Robust Mean: 10.3 ug/L
Std Dev: 3.2537 ug/L
Median: 10.4 ug/L

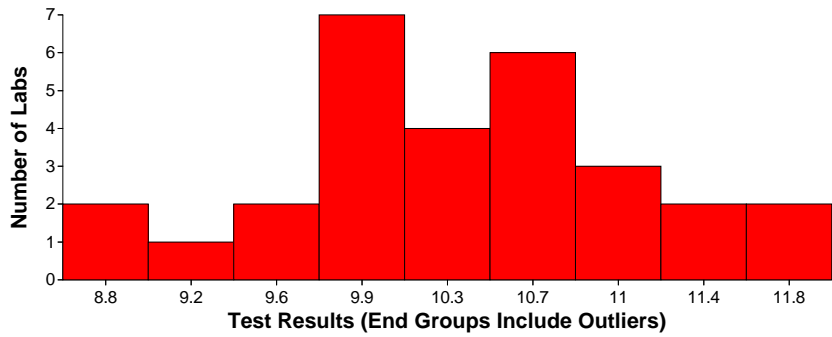

Totals for Matrix/Analyte/Technology:

Labs: Pass: 26 Fail: 3 Total: 29

Totals for Matrix/Analyte: Labs: Pass: 27 Fail: 3 Total: 30

Potable Water 1,1,2,2-Tetrachloroethane

Shipment: 407 Matrix: Potable Water
Analyte: 1,1,2,2-Tetrachloroethane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 10.3 ug/L
Limits: 8.24 to 12.4 ug/L
Basis: Fixed Percent (2)
Robust Mean: 9.8 ug/L
Std Dev: 0 ug/L
Median: 9.79 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 27 Fail: 3 Total: 30

Potable Water 1,1,2-Trichloroethane

Shipment: 407 Matrix: Potable Water
Analyte: 1,1,2-Trichloroethane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 7.25 ug/L
Limits: 4.35 to 10.2 ug/L
Basis: Fixed Percent (2)
Robust Mean: 7.2 ug/L
Std Dev: 1.4488 ug/L
Median: 7.17 ug/L

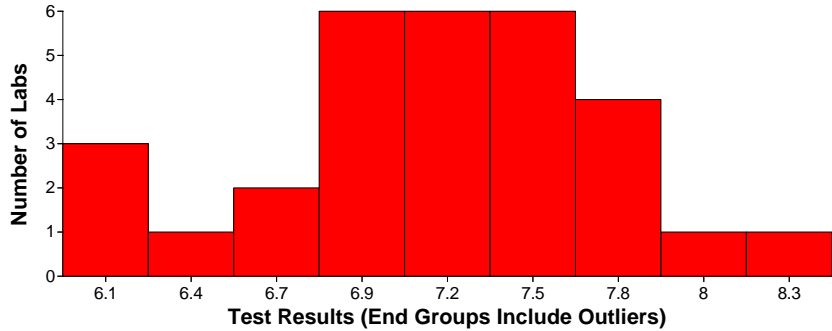

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water 1,1,2-Trichloroethane

Shipment: 407 Matrix: Potable Water
Analyte: 1,1,2-Trichloroethane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 7.25 ug/L
Limits: 4.35 to 10.2 ug/L
Basis: Fixed Percent (2)
Robust Mean: 7.2 ug/L
Std Dev: 0 ug/L
Median: 7.15 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water 1,1-Dichloroethane

Potable Water 1,1-Dichloroethane

Shipment: 407 Matrix: Potable Water
Analyte: 1,1-Dichloroethane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 4.82 ug/L
Limits: 2.89 to 6.75 ug/L
Basis: Fixed Percent (2)
Robust Mean: 5 ug/L
Std Dev: 0.9733 ug/L
Median: 5.04 ug/L

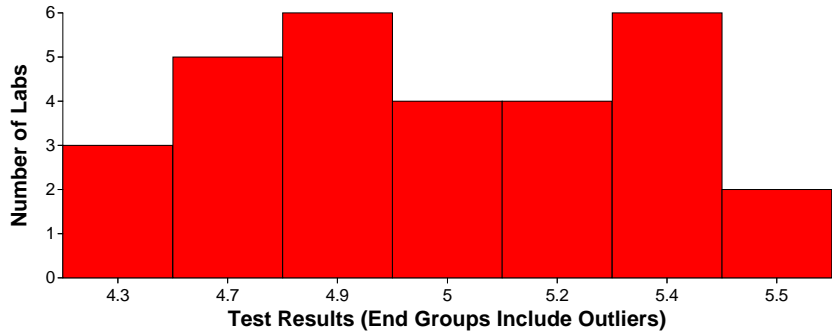

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water 1,1-Dichloroethane

Shipment: 407 Matrix: Potable Water
Analyte: 1,1-Dichloroethane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 4.82 ug/L
Limits: 2.89 to 6.75 ug/L
Basis: Fixed Percent (2)
Robust Mean: 5.1 ug/L
Std Dev: 0 ug/L
Median: 5.14 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water 1,1-Dichloroethene

Shipment: 407 Matrix: Potable Water
Analyte: 1,1-Dichloroethene
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 16.8 ug/L
Limits: 13.4 to 20.2 ug/L
Basis: Fixed Percent (2)
Robust Mean: 16.9 ug/L
Std Dev: 4.5784 ug/L
Median: 17.15 ug/L

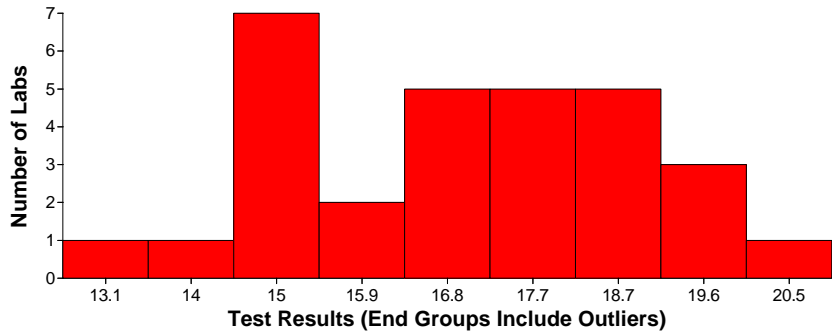

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 2 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water 1,1-Dichloroethene

Shipment: 407 Matrix: Potable Water
Analyte: 1,1-Dichloroethene
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 16.8 ug/L
Limits: 13.4 to 20.2 ug/L
Basis: Fixed Percent (2)
Robust Mean: 14.8 ug/L
Std Dev: 0 ug/L
Median: 14.8 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water 1,1-Dichloropropene

Potable Water 1,1-Dichloropropene

Shipment: 407 Matrix: Potable Water
Analyte: 1,1-Dichloropropene
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 5.78 ug/L
Limits: 3.47 to 8.09 ug/L
Basis: Fixed Percent (2)
Robust Mean: 5.9 ug/L
Std Dev: 1.6115 ug/L
Median: 5.97 ug/L

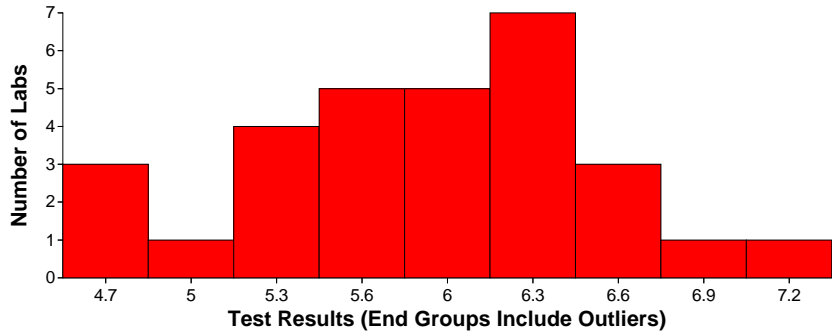

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water 1,1-Dichloropropene

Shipment: 407 Matrix: Potable Water
Analyte: 1,1-Dichloropropene
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 5.78 ug/L
Limits: 3.47 to 8.09 ug/L
Basis: Fixed Percent (2)
Robust Mean: 6.4 ug/L
Std Dev: 0 ug/L
Median: 6.38 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water 1,2,3-Trichloropropane

Shipment: 407 Matrix: Potable Water
Analyte: 1,2,3-Trichloropropane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 15.6 ug/L
Limits: 12.5 to 18.7 ug/L
Basis: Fixed Percent (2)
Robust Mean: 15.2 ug/L
Std Dev: 4.0679 ug/L
Median: 15.1 ug/L

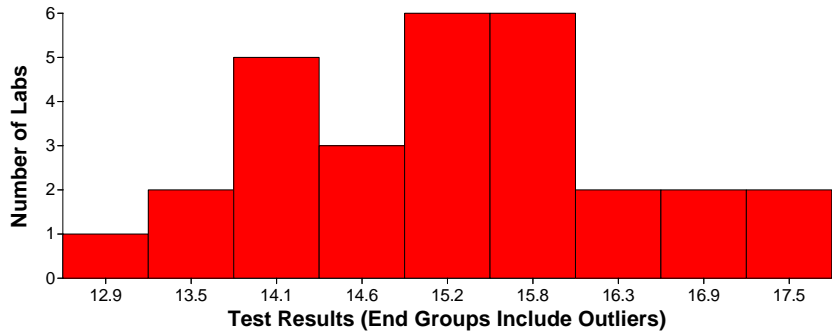

Totals for Matrix/Analyte/Technology:

Labs: Pass: 27 Fail: 2 Total: 29

Totals for Matrix/Analyte: Labs: Pass: 28 Fail: 2 Total: 30

Potable Water 1,2,3-Trichloropropane

Shipment: 407 Matrix: Potable Water
Analyte: 1,2,3-Trichloropropane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 15.6 ug/L
Limits: 12.5 to 18.7 ug/L
Basis: Fixed Percent (2)
Robust Mean: 16.1 ug/L
Std Dev: 0 ug/L
Median: 16.1 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 28 Fail: 2 Total: 30

Potable Water 1,2,4-Trichlorobenzene

Potable Water 1,2,4-Trichlorobenzene

Shipment: 407 Matrix: Potable Water
Analyte: 1,2,4-Trichlorobenzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 12.5 ug/L
Limits: 10 to 15 ug/L
Basis: Fixed Percent (2)
Robust Mean: 12.5 ug/L
Std Dev: 2.5778 ug/L
Median: 12.2 ug/L

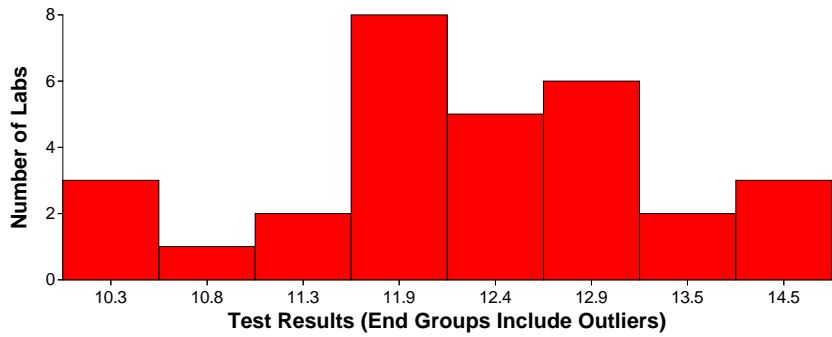

Totals for Matrix/Analyte/Technology:

Labs: Pass: 27 Fail: 3 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 28 Fail: 3 Total: 31

Potable Water 1,2,4-Trichlorobenzene

Shipment: 407 Matrix: Potable Water
Analyte: 1,2,4-Trichlorobenzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 12.5 ug/L
Limits: 10 to 15 ug/L
Basis: Fixed Percent (2)
Robust Mean: 11.9 ug/L
Std Dev: 0 ug/L
Median: 11.9 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 28 Fail: 3 Total: 31

Potable Water 1,2,4-Trimethylbenzene

Shipment: 407 Matrix: Potable Water
Analyte: 1,2,4-Trimethylbenzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 14.3 ug/L
Limits: 11.4 to 17.2 ug/L
Basis: Fixed Percent (2)
Robust Mean: 14.2 ug/L
Std Dev: 3.7266 ug/L
Median: 14 ug/L

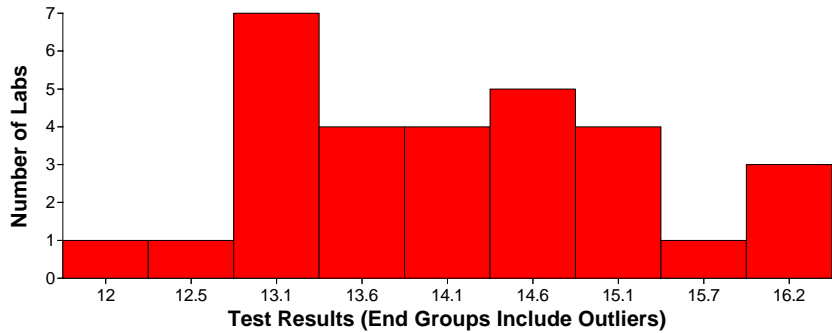

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 2 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water 1,2,4-Trimethylbenzene

Shipment: 407 Matrix: Potable Water
Analyte: 1,2,4-Trimethylbenzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 14.3 ug/L
Limits: 11.4 to 17.2 ug/L
Basis: Fixed Percent (2)
Robust Mean: 13.1 ug/L
Std Dev: 0 ug/L
Median: 13.1 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water 1,2-Dibromo-3-chloropropane

Potable Water 1,2-Dibromo-3-chloropropane


Shipment: 407 **Matrix:** Potable Water
Analyte: 1,2-Dibromo-3-chloropropane
Sample: 0722
Technology: GC-ECD
Prep Method:
Target: 0.303 ug/L
Limits: 0.182 to 0.424 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 0.3 ug/L
Std Dev: 0.0978 ug/L
Median: 0.305 ug/L

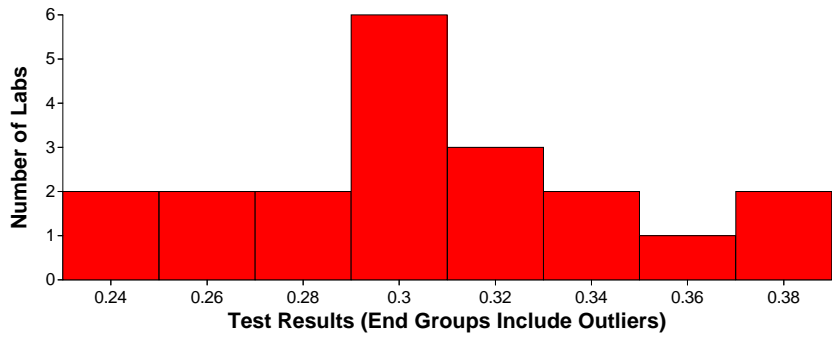

Totals for Matrix/Analyte/Technology:
Labs: Pass: 18 **Fail:** 2 **Total:** 20
Totals for Matrix/Analyte: **Labs: Pass:** 18 **Fail:** 2 **Total:** 20

Potable Water 1,2-Dichloroethane

Shipment: 407 **Matrix:** Potable Water
Analyte: 1,2-Dichloroethane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 5.67 ug/L
Limits: 3.4 to 7.94 ug/L
Basis: Fixed Percent (2)
Robust Mean: 5.8 ug/L
Std Dev: 1.1142 ug/L
Median: 5.77 ug/L

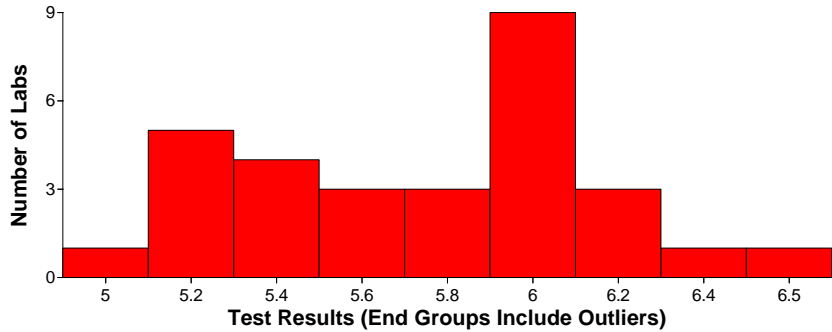

Totals for Matrix/Analyte/Technology:
Labs: Pass: 29 **Fail:** 1 **Total:** 30
Totals for Matrix/Analyte: **Labs: Pass:** 30 **Fail:** 1 **Total:** 31

Potable Water 1,2-Dichloroethane


Shipment: 407 **Matrix:** Potable Water
Analyte: 1,2-Dichloroethane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 5.67 ug/L
Limits: 3.4 to 7.94 ug/L
Basis: Fixed Percent (2)
Robust Mean: 6.1 ug/L
Std Dev: 0 ug/L
Median: 6.05 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
Labs: Pass: 1 **Fail:** 0 **Total:** 1
Totals for Matrix/Analyte: **Labs: Pass:** 30 **Fail:** 1 **Total:** 31

Potable Water 1,2-Dichlorobenzene

Shipment: 407 **Matrix:** Potable Water
Analyte: 1,2-Dichlorobenzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 14 ug/L
Limits: 11.2 to 16.8 ug/L
Basis: Fixed Percent (2)
Robust Mean: 14.2 ug/L
Std Dev: 3.6892 ug/L
Median: 13.95 ug/L

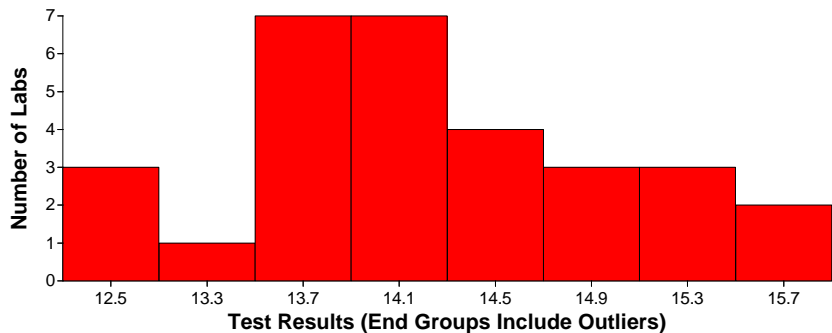

Totals for Matrix/Analyte/Technology:
Labs: Pass: 29 **Fail:** 1 **Total:** 30
Totals for Matrix/Analyte: **Labs: Pass:** 30 **Fail:** 1 **Total:** 31

Potable Water 1,2-Dichlorobenzene

Shipment: 407 Matrix: Potable Water
Analyte: 1,2-Dichlorobenzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 14 ug/L
Limits: 11.2 to 16.8 ug/L
Basis: Fixed Percent (2)
Robust Mean: 13.7 ug/L
Std Dev: 0 ug/L
Median: 13.7 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water cis-1,2-Dichloroethene

Shipment: 407 Matrix: Potable Water
Analyte: cis-1,2-Dichloroethene
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 12.6 ug/L
Limits: 10.1 to 15.1 ug/L
Basis: Fixed Percent (2)
Robust Mean: 12.8 ug/L
Std Dev: 3.9694 ug/L
Median: 12.75 ug/L

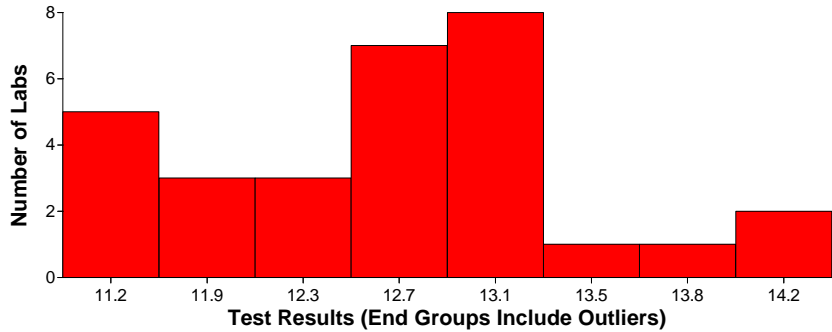

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 2 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water cis-1,2-Dichloroethene

Shipment: 407 Matrix: Potable Water
Analyte: cis-1,2-Dichloroethene
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 12.6 ug/L
Limits: 10.1 to 15.1 ug/L
Basis: Fixed Percent (2)
Robust Mean: 12.5 ug/L
Std Dev: 0 ug/L
Median: 12.5 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water 1,2-Dichloropropane

Shipment: 407 Matrix: Potable Water
Analyte: 1,2-Dichloropropane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 17.5 ug/L
Limits: 14 to 21 ug/L
Basis: Fixed Percent (2)
Robust Mean: 17.6 ug/L
Std Dev: 3.4603 ug/L
Median: 17.8 ug/L

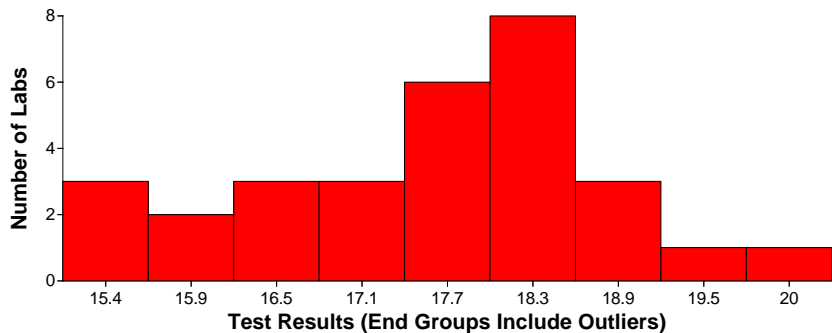

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water 1,2-Dichloropropane

Shipment: 407 Matrix: Potable Water
Analyte: 1,2-Dichloropropane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 17.5 ug/L
Limits: 14 to 21 ug/L
Basis: Fixed Percent (2)
Robust Mean: 16.6 ug/L
Std Dev: 0 ug/L
Median: 16.6 ug/L

A histogram is not displayed for
Technology: GCELCD/PID due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water 1,2-Dibromoethane

Shipment: 407 Matrix: Potable Water
Analyte: 1,2-Dibromoethane
Sample: 0722
Technology: GC-ECD
Prep Method:
Target: 1.1 ug/L
Limits: 0.66 to 1.54 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 1.1 ug/L
Std Dev: 0.3425 ug/L
Median: 1.085 ug/L

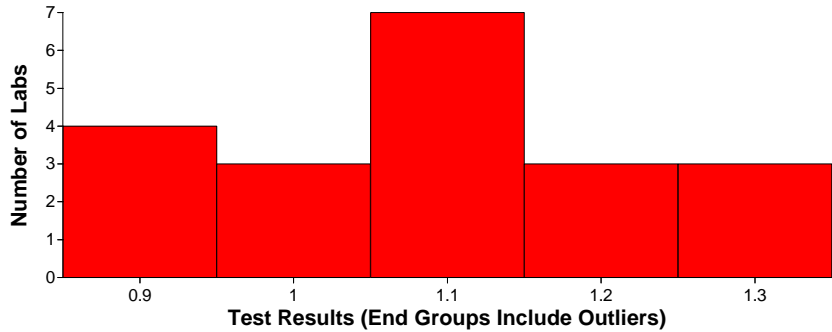


Totals for Matrix/Analyte/Technology:

Labs: Pass: 19 Fail: 1 Total: 20

Totals for Matrix/Analyte: Labs: Pass: 19 Fail: 1 Total: 20

Potable Water 1,3-Dichlorobenzene

Shipment: 407 Matrix: Potable Water
Analyte: 1,3-Dichlorobenzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 13.8 ug/L
Limits: 11 to 16.6 ug/L
Basis: Fixed Percent (2)
Robust Mean: 13.9 ug/L
Std Dev: 3.6727 ug/L
Median: 14 ug/L

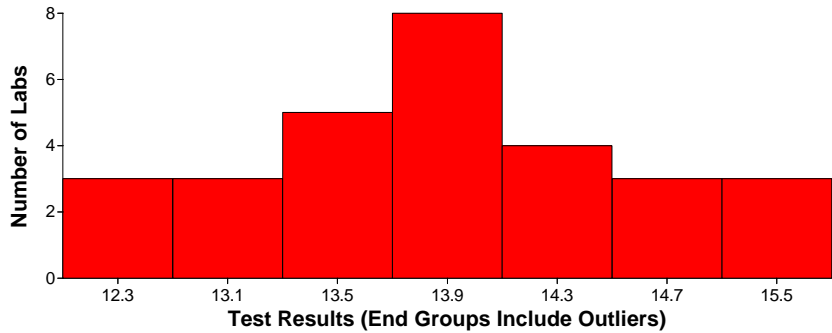

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 1 Total: 29

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 1 Total: 30

Potable Water 1,3-Dichlorobenzene

Shipment: 407 Matrix: Potable Water
Analyte: 1,3-Dichlorobenzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 13.8 ug/L
Limits: 11 to 16.6 ug/L
Basis: Fixed Percent (2)
Robust Mean: 13.4 ug/L
Std Dev: 0 ug/L
Median: 13.4 ug/L

A histogram is not displayed for
Technology: GCELCD/PID due to the
limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 1 Total: 30

Potable Water 1,3-Dichloropropane

Potable Water 1,3-Dichloropropane

Shipment: 407 Matrix: Potable Water
Analyte: 1,3-Dichloropropane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 13.5 ug/L
Limits: 10.8 to 16.2 ug/L
Basis: Fixed Percent (2)
Robust Mean: 13.5 ug/L
Std Dev: 2.5975 ug/L
Median: 13.6 ug/L

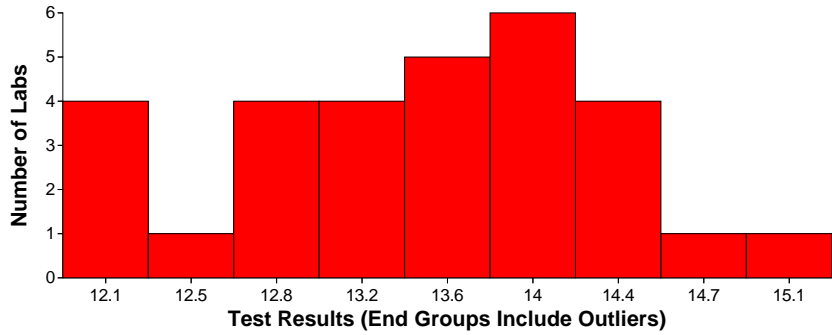

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water 1,3-Dichloropropane

Shipment: 407 Matrix: Potable Water
Analyte: 1,3-Dichloropropane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 13.5 ug/L
Limits: 10.8 to 16.2 ug/L
Basis: Fixed Percent (2)
Robust Mean: 13.6 ug/L
Std Dev: 0 ug/L
Median: 13.6 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water 1,4-Dichlorobenzene

Shipment: 407 Matrix: Potable Water
Analyte: 1,4-Dichlorobenzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 2.44 ug/L
Limits: 1.46 to 3.42 ug/L
Basis: Fixed Percent (2)
Robust Mean: 2.5 ug/L
Std Dev: 0.8069 ug/L
Median: 2.465 ug/L

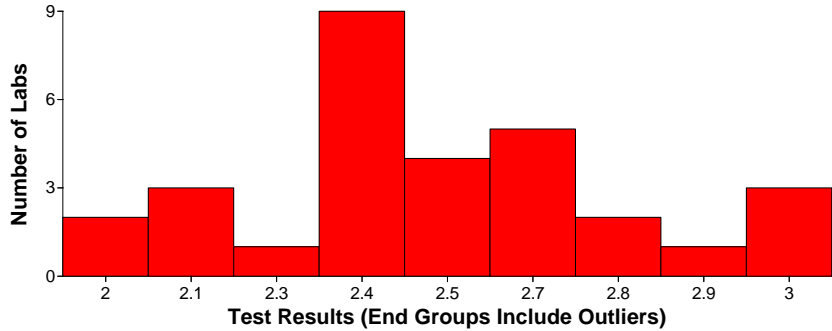

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 2 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water 1,4-Dichlorobenzene

Shipment: 407 Matrix: Potable Water
Analyte: 1,4-Dichlorobenzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 2.44 ug/L
Limits: 1.46 to 3.42 ug/L
Basis: Fixed Percent (2)
Robust Mean: 2.6 ug/L
Std Dev: 0 ug/L
Median: 2.62 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water 2,2-Dichloropropane

Potable Water 2,2-Dichloropropane

Shipment: 407 Matrix: Potable Water
Analyte: 2,2-Dichloropropane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 6.55 ug/L
Limits: 3.93 to 9.17 ug/L
Basis: Fixed Percent (2)
Robust Mean: 6.2 ug/L
Std Dev: 1.0109 ug/L
Median: 6.3 ug/L

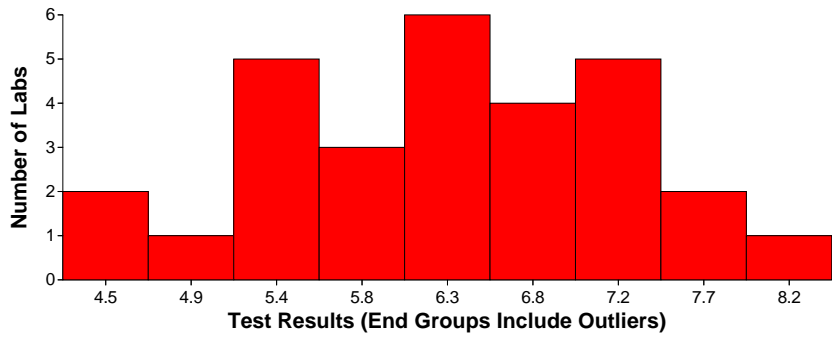

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 1 Total: 29

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 1 Total: 30

Potable Water 2,2-Dichloropropane

Shipment: 407 Matrix: Potable Water
Analyte: 2,2-Dichloropropane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 6.55 ug/L
Limits: 3.93 to 9.17 ug/L
Basis: Fixed Percent (2)
Robust Mean: 6.3 ug/L
Std Dev: 0 ug/L
Median: 6.29 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 1 Total: 30

Potable Water 2,4-D

Shipment: 407 Matrix: Potable Water
Analyte: 2,4-D
Sample: 0717
Technology: GC-ECD
Prep Method:
Target: 35 ug/L
Limits: 17.5 to 52.5 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 31.4 ug/L
Std Dev: 5.9209 ug/L
Median: 32.05 ug/L

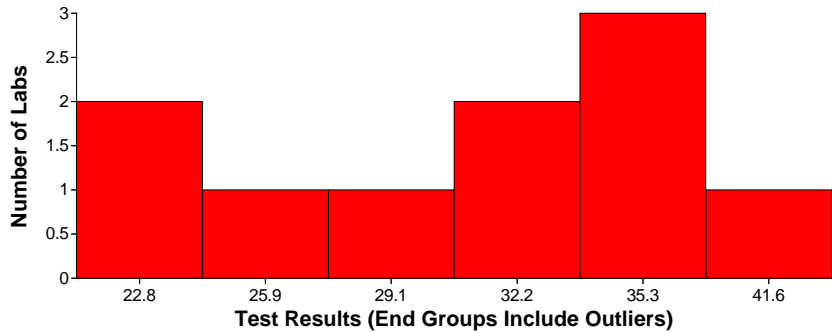

Totals for Matrix/Analyte/Technology:

Labs: Pass: 10 Fail: 0 Total: 10

Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water 2,4-D

Shipment: 407 Matrix: Potable Water
Analyte: 2,4-D
Sample: 0717
Technology: HPLC-UV
Prep Method:
Target: 35 ug/L
Limits: 17.5 to 52.5 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 39.4 ug/L
Std Dev: 0 ug/L
Median: 39.4 ug/L

A histogram is not displayed for Technology: HPLC-UV due to the limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water 3-Hydroxy Carbofuran

Potable Water 3-Hydroxy Carbofuran

Shipment: 407 Matrix: Potable Water
Analyte: 3-Hydroxy Carbofuran
Sample: 0715
Technology: HPLC-FLUOR
Prep Method:
Target: 71.6 ug/L
Limits: 57.3 to 85.9 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 68.3 ug/L
Std Dev: 4.1281 ug/L
Median: 68.4 ug/L

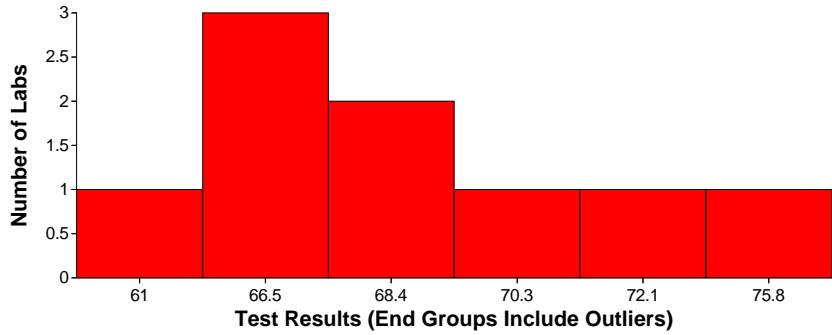

Totals for Matrix/Analyte/Technology:
Labs: Pass: 9 Fail: 0 Total: 9
Totals for Matrix/Analyte: Labs: Pass: 9 Fail: 0 Total: 9

Potable Water Acifluorofen

Shipment: 407 Matrix: Potable Water
Analyte: Acifluorofen
Sample: 0717
Technology: GC-ECD
Prep Method:
Target: 55.9 ug/L
Limits: 28 to 83.9 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 59.3 ug/L
Std Dev: 7.9196 ug/L
Median: 59.3 ug/L

A histogram is not displayed for Technology: GC-ECD due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
Labs: Pass: 2 Fail: 0 Total: 2
Totals for Matrix/Analyte: Labs: Pass: 3 Fail: 0 Total: 3

Potable Water Acifluorofen


Shipment: 407 Matrix: Potable Water
Analyte: Acifluorofen
Sample: 0717
Technology: HPLC-UV
Prep Method:
Target: 55.9 ug/L
Limits: 28 to 83.9 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 60.2 ug/L
Std Dev: 0 ug/L
Median: 60.2 ug/L

A histogram is not displayed for Technology: HPLC-UV due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
Labs: Pass: 1 Fail: 0 Total: 1
Totals for Matrix/Analyte: Labs: Pass: 3 Fail: 0 Total: 3

Potable Water Silver, Total

Shipment: 407 Matrix: Potable Water
Analyte: Silver, Total
Sample: 0706
Technology: FAAS
Prep Method:
Target: 139 ug/L
Limits: 97.3 to 181 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 141 ug/L
Std Dev: 7.8102 ug/L
Median: 137 ug/L

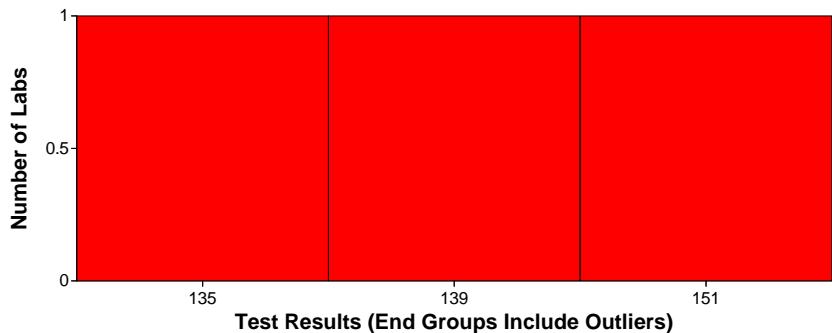


Totals for Matrix/Analyte/Technology:
Labs: Pass: 3 Fail: 0 Total: 3
Totals for Matrix/Analyte: Labs: Pass: 53 Fail: 1 Total: 54

Potable Water Silver, Total

Potable Water Silver, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Silver, Total
 Sample: 0706
 Technology: GFAAS
 Prep Method:
 Target: 139 ug/L
 Limits: 97.3 to 181 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 128 ug/L
 Std Dev: 73.9008 ug/L
 Median: 128 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 3 Fail: 0 Total: 3
 Totals for Matrix/Analyte: Labs: Pass: 53 Fail: 1 Total: 54

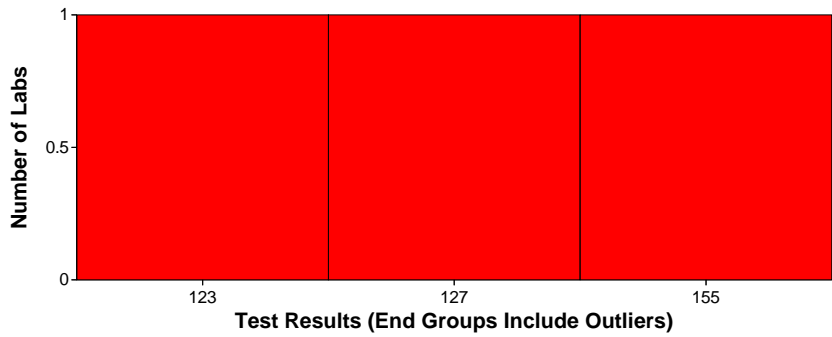

Potable Water Silver, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Silver, Total
 Sample: 0706
 Technology: ICP-AES
 Prep Method:
 Target: 139 ug/L
 Limits: 97.3 to 181 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 141.3 ug/L
 Std Dev: 30.2539 ug/L
 Median: 141 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 23 Fail: 0 Total: 23
 Totals for Matrix/Analyte: Labs: Pass: 53 Fail: 1 Total: 54

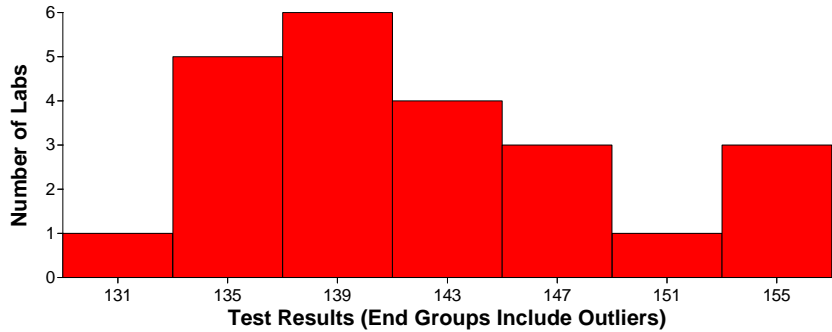

Potable Water Silver, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Silver, Total
 Sample: 0706
 Technology: ICP-MS
 Prep Method:
 Target: 139 ug/L
 Limits: 97.3 to 181 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 137.3 ug/L
 Std Dev: 28.205 ug/L
 Median: 135 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 24 Fail: 1 Total: 25
 Totals for Matrix/Analyte: Labs: Pass: 53 Fail: 1 Total: 54

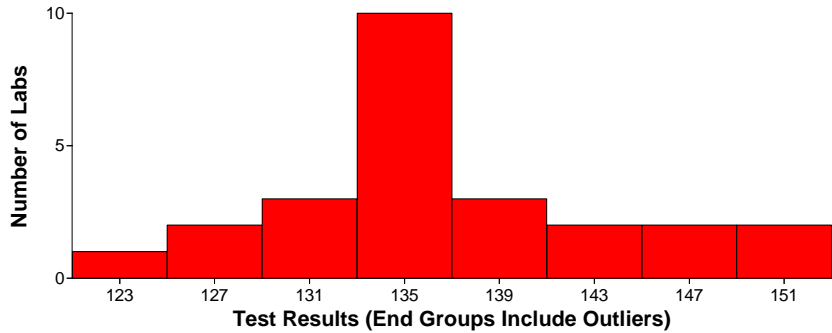

Potable Water Aluminum, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Aluminum, Total
 Sample: 0706
 Technology: ICP-AES
 Prep Method:
 Target: 900 ug/L
 Limits: 765 to 1040 ug/L
 Basis: Fixed Percent (2)
 Robust Mean: 867.2 ug/L
 Std Dev: 190.4638 ug/L
 Median: 875.5 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 21 Fail: 1 Total: 22
 Totals for Matrix/Analyte: Labs: Pass: 41 Fail: 3 Total: 44

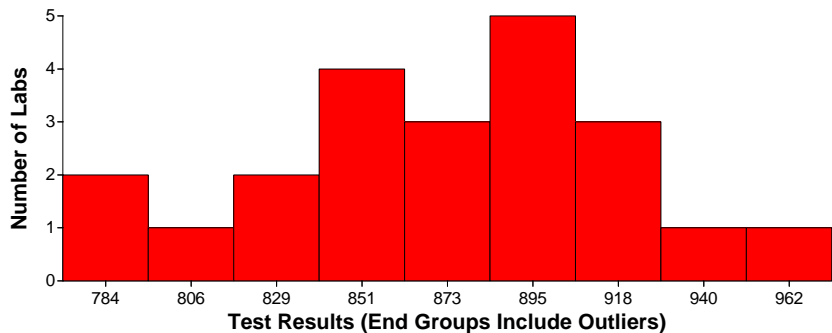

Potable Water Aluminum, Total

Potable Water Aluminum, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Aluminum, Total
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 900 ug/L
Limits: 765 to 1040 ug/L
Basis: Fixed Percent (2)
Robust Mean: 875.9 ug/L
Std Dev: 260.7712 ug/L
Median: 873 ug/L

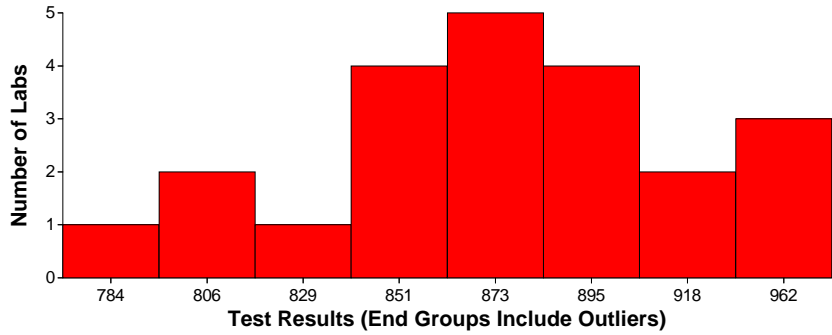


Totals for Matrix/Analyte/Technology:
Labs: Pass: 20 **Fail:** 2 **Total:** 22

Totals for Matrix/Analyte: **Labs: Pass:** 41 **Fail:** 3 **Total:** 44

Potable Water Alachlor

Shipment: 407 **Matrix:** Potable Water
Analyte: Alachlor
Sample: 0707B
Technology: GC-ECD
Prep Method:
Target: 16.7 ug/L
Limits: 9.19 to 24.2 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 16.1 ug/L
Std Dev: 0.6716 ug/L
Median: 15.85 ug/L

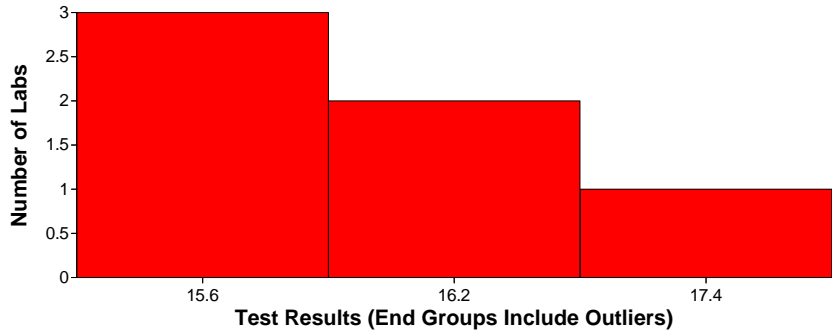


Totals for Matrix/Analyte/Technology:
Labs: Pass: 6 **Fail:** 0 **Total:** 6

Totals for Matrix/Analyte: **Labs: Pass:** 16 **Fail:** 0 **Total:** 16

Potable Water Alachlor

Shipment: 407 **Matrix:** Potable Water
Analyte: Alachlor
Sample: 0707B
Technology: GC-MS
Prep Method:
Target: 16.7 ug/L
Limits: 9.19 to 24.2 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 16.7 ug/L
Std Dev: 5.5245 ug/L
Median: 16.35 ug/L

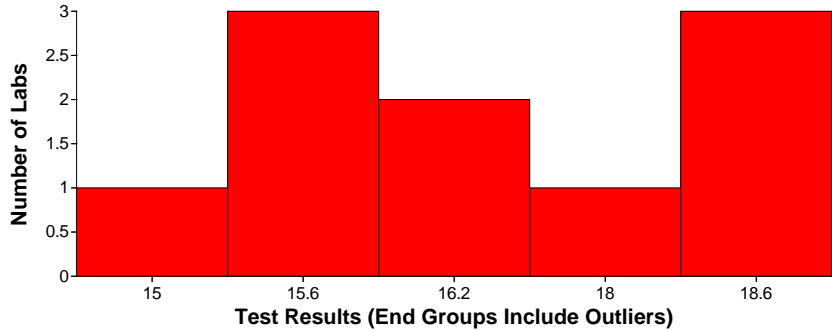


Totals for Matrix/Analyte/Technology:
Labs: Pass: 10 **Fail:** 0 **Total:** 10

Totals for Matrix/Analyte: **Labs: Pass:** 16 **Fail:** 0 **Total:** 16

Potable Water Aldicarb

Shipment: 407 **Matrix:** Potable Water
Analyte: Aldicarb
Sample: 0715
Technology: HPLC-FLUOR
Prep Method:
Target: 22.7 ug/L
Limits: 17 to 28.4 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 23.5 ug/L
Std Dev: 1.7992 ug/L
Median: 22.77 ug/L

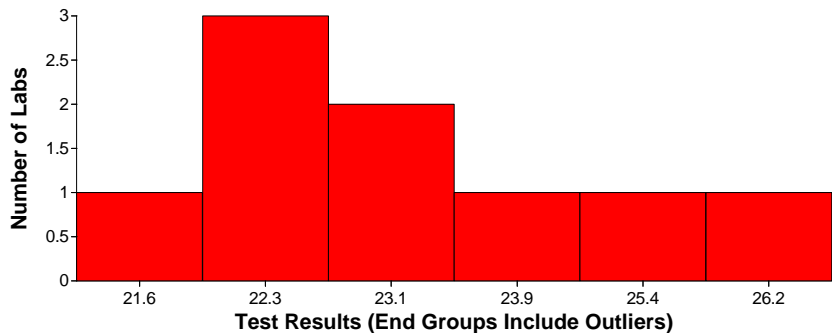

Totals for Matrix/Analyte/Technology:
Labs: Pass: 9 **Fail:** 0 **Total:** 9


Totals for Matrix/Analyte: **Labs: Pass:** 9 **Fail:** 0 **Total:** 9

Potable Water Aldrin

Potable Water Aldrin

Shipment: 407 **Matrix:** Potable Water
Analyte: Aldrin
Sample: 0707A
Technology: GC-ECD
Prep Method:
Target: 2.35 ug/L
Limits: 1.06 to 2.99 ug/L
Basis: Linear Regression
Robust Mean: 2.1 ug/L
Std Dev: 0.6435 ug/L
Median: 2.13 ug/L


Totals for Matrix/Analyte/Technology:
Labs: Pass: 10 **Fail:** 1 **Total:** 11
Totals for Matrix/Analyte: **Labs: Pass:** 17 **Fail:** 1 **Total:** 18

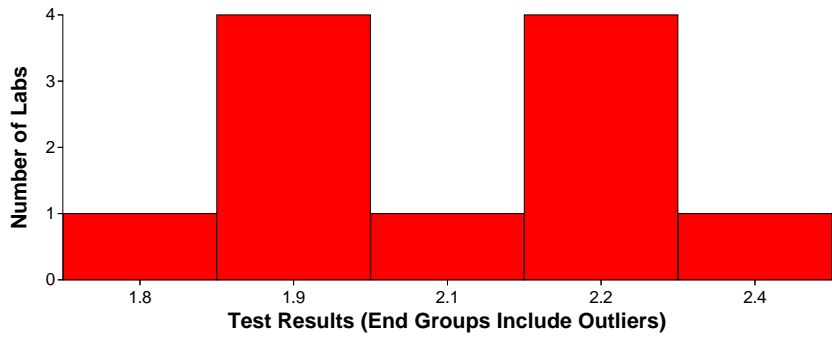

Potable Water Aldrin

Shipment: 407 **Matrix:** Potable Water
Analyte: Aldrin
Sample: 0707A
Technology: GC-MS
Prep Method:
Target: 2.35 ug/L
Limits: 1.06 to 2.99 ug/L
Basis: Linear Regression
Robust Mean: 2 ug/L
Std Dev: 0.2343 ug/L
Median: 1.94 ug/L


Totals for Matrix/Analyte/Technology:
Labs: Pass: 7 **Fail:** 0 **Total:** 7
Totals for Matrix/Analyte: **Labs: Pass:** 17 **Fail:** 1 **Total:** 18

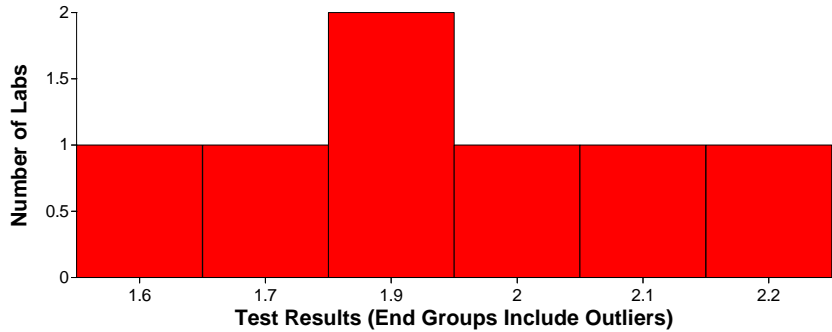

Potable Water Aldicarb Sulfone

Shipment: 407 **Matrix:** Potable Water
Analyte: Aldicarb Sulfone
Sample: 0715
Technology: HPLC-FLUOR
Prep Method:
Target: 42.5 ug/L
Limits: 31.9 to 53.1 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 41.7 ug/L
Std Dev: 2.6143 ug/L
Median: 41.7 ug/L

Totals for Matrix/Analyte/Technology:
Labs: Pass: 9 **Fail:** 0 **Total:** 9
Totals for Matrix/Analyte: **Labs: Pass:** 9 **Fail:** 0 **Total:** 9

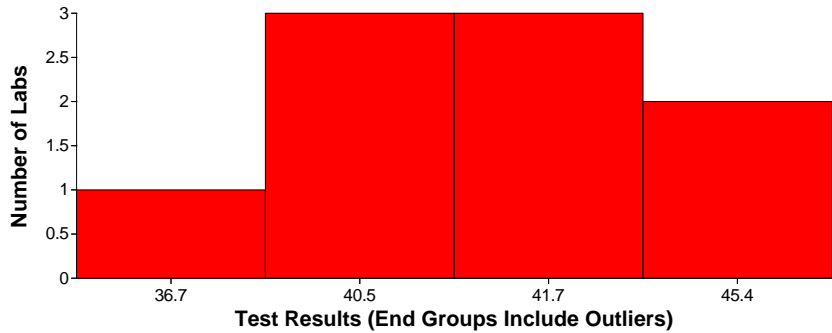

Potable Water Alkalinity

Shipment: 407 **Matrix:** Potable Water
Analyte: Alkalinity
Sample: 0701
Technology: COLOR
Prep Method:
Target: 79.8 mg/L
Limits: 71.8 to 87.8 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 78 mg/L
Std Dev: 6.8589 mg/L
Median: 77.95 mg/L


Totals for Matrix/Analyte/Technology:
Labs: Pass: 2 **Fail:** 0 **Total:** 2
Totals for Matrix/Analyte: **Labs: Pass:** 51 **Fail:** 3 **Total:** 54

A histogram is not displayed for Technology: COLOR due to the limited number of participants.

Potable Water Alkalinity

Potable Water Alkalinity


Shipment: 407 **Matrix:** Potable Water
Analyte: Alkalinity
Sample: 0701
Technology: TITR
Prep Method:
Target: 79.8 mg/L
Limits: 71.8 to 87.8 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 78.8 mg/L
Std Dev: 15.5974 mg/L
Median: 78.8 mg/L

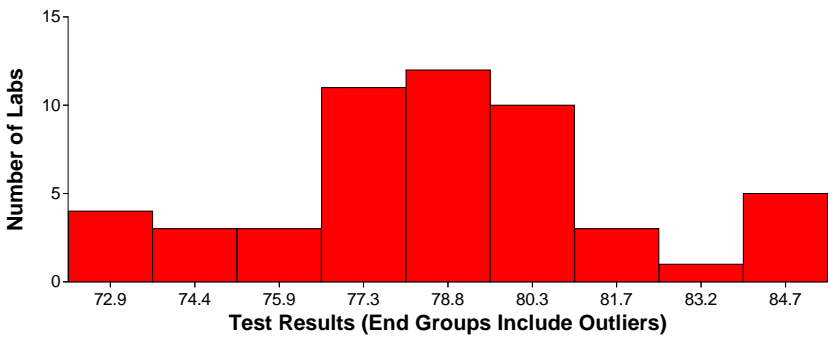

Totals for Matrix/Analyte/Technology:
Labs: Pass: 49 **Fail:** 3 **Total:** 52
Totals for Matrix/Analyte: **Labs: Pass:** 51 **Fail:** 3 **Total:** 54

Potable Water Arsenic, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Arsenic, Total
Sample: 0706
Technology: GFAAS
Prep Method:
Target: 45.1 ug/L
Limits: 31.6 to 58.6 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 44.1 ug/L
Std Dev: 2.9436 ug/L
Median: 45.05 ug/L

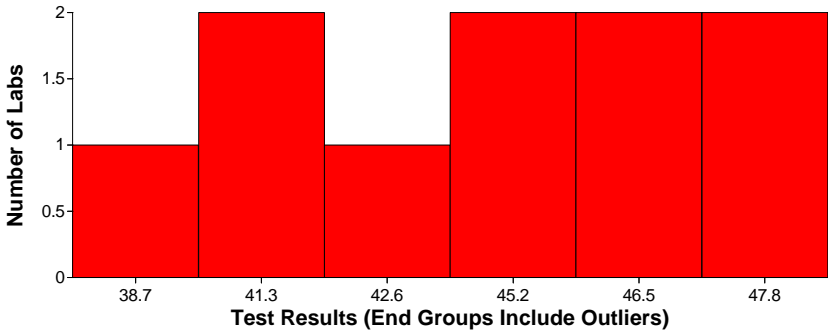

Totals for Matrix/Analyte/Technology:
Labs: Pass: 10 **Fail:** 0 **Total:** 10
Totals for Matrix/Analyte: **Labs: Pass:** 39 **Fail:** 1 **Total:** 40

Potable Water Arsenic, Total


Shipment: 407 **Matrix:** Potable Water
Analyte: Arsenic, Total
Sample: 0706
Technology: ICP-AES
Prep Method:
Target: 45.1 ug/L
Limits: 31.6 to 58.6 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 42.5 ug/L
Std Dev: 3.0406 ug/L
Median: 42.45 ug/L

A histogram is not displayed for Technology: ICP-AES due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
Labs: Pass: 2 **Fail:** 0 **Total:** 2
Totals for Matrix/Analyte: **Labs: Pass:** 39 **Fail:** 1 **Total:** 40

Potable Water Arsenic, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Arsenic, Total
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 45.1 ug/L
Limits: 31.6 to 58.6 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 43.8 ug/L
Std Dev: 8.6327 ug/L
Median: 44.1 ug/L

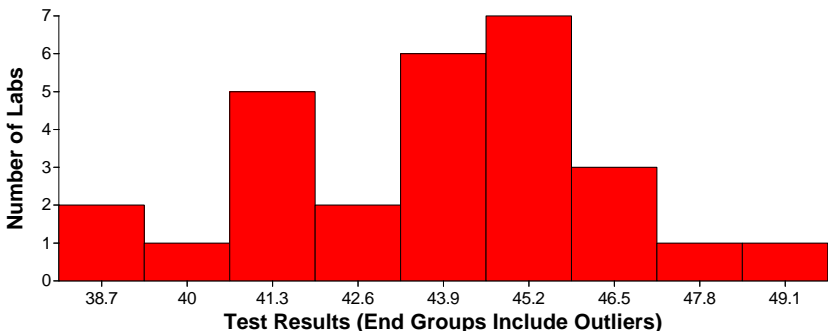


Totals for Matrix/Analyte/Technology:
Labs: Pass: 27 **Fail:** 1 **Total:** 28
Totals for Matrix/Analyte: **Labs: Pass:** 39 **Fail:** 1 **Total:** 40

Potable Water Atrazine

Potable Water Atrazine

Shipment: 407 Matrix: Potable Water
 Analyte: Atrazine
 Sample: 0707B
 Technology: GC-ECD
 Prep Method:
 Target: 16.5 ug/L
 Limits: 9.08 to 23.9 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 15.9 ug/L
 Std Dev: 1.6289 ug/L
 Median: 15.2 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 3 Fail: 0 Total: 3
 Totals for Matrix/Analyte: Labs: Pass: 14 Fail: 0 Total: 14

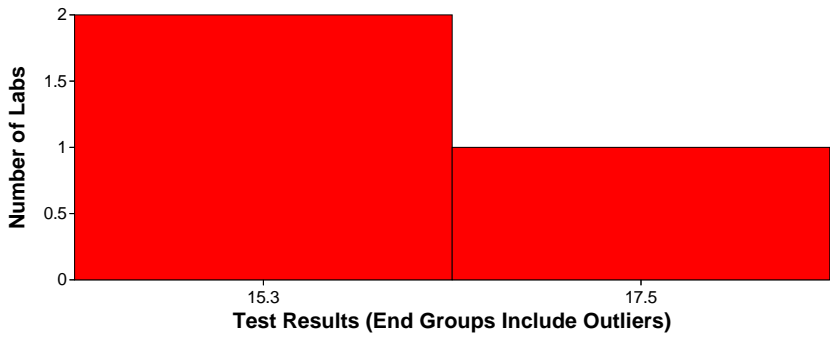

Potable Water Atrazine

Shipment: 407 Matrix: Potable Water
 Analyte: Atrazine
 Sample: 0707B
 Technology: GC-MS
 Prep Method:
 Target: 16.5 ug/L
 Limits: 9.08 to 23.9 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 16.6 ug/L
 Std Dev: 2.6655 ug/L
 Median: 17 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 11 Fail: 0 Total: 11
 Totals for Matrix/Analyte: Labs: Pass: 14 Fail: 0 Total: 14

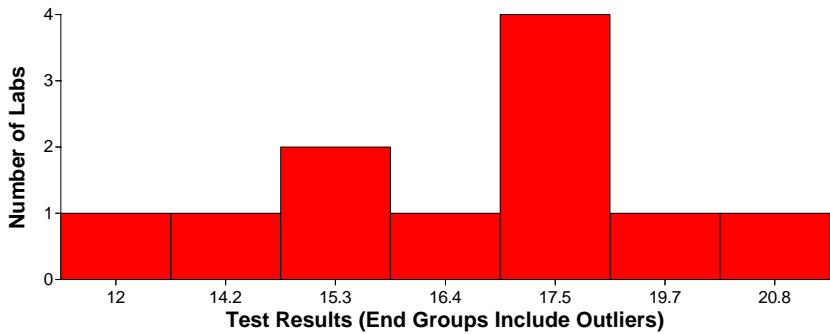

Potable Water Di (2-ethylhexyl) adipate

Shipment: 407 Matrix: Potable Water
 Analyte: Di (2-ethylhexyl) adipate
 Sample: 0708
 Technology: GC-MS
 Prep Method:
 Target: 21.4 ug/L
 Limits: 12.3 to 28.9 ug/L
 Basis: Linear Regression
 Robust Mean: 20.2 ug/L
 Std Dev: 5.3813 ug/L
 Median: 20.3 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 11 Fail: 2 Total: 13
 Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 2 Total: 13

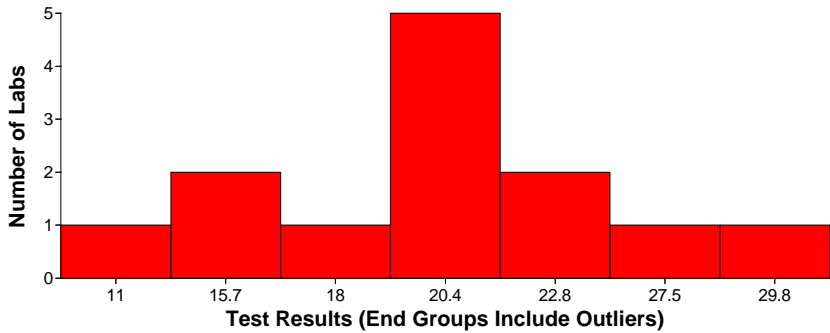

Potable Water Bis(2-ethylhexyl) phthalate

Shipment: 407 Matrix: Potable Water
 Analyte: Bis(2-ethylhexyl) phthalate
 Sample: 0708
 Technology: GC-MS
 Prep Method:
 Target: 27.4 ug/L
 Limits: 13.9 to 39.3 ug/L
 Basis: Linear Regression
 Robust Mean: 25.5 ug/L
 Std Dev: 6.4971 ug/L
 Median: 26.5 ug/L

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 12 Fail: 1 Total: 13
 Totals for Matrix/Analyte: Labs: Pass: 12 Fail: 1 Total: 13

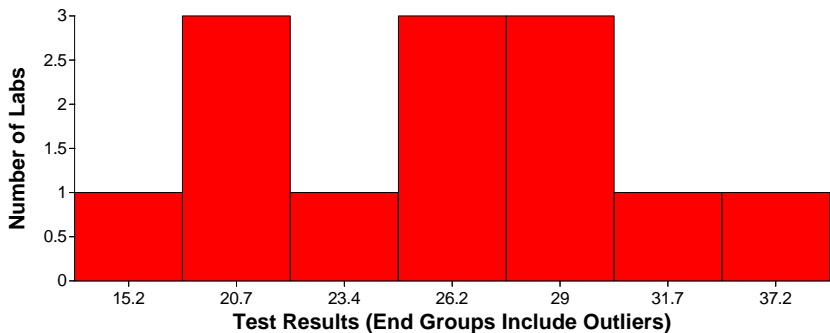


Potable Water Barium, Total

Potable Water Barium, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Barium, Total
 Sample: 0706
 Technology: ICP-AES
 Prep Method:
 Target: 1950 ug/L
 Limits: 1660 to 2240 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 1946.4 ug/L
 Std Dev: 553.8231 ug/L
 Median: 1950 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 22 Fail: 2 Total: 24
 Totals for Matrix/Analyte: Labs: Pass: 49 Fail: 3 Total: 52

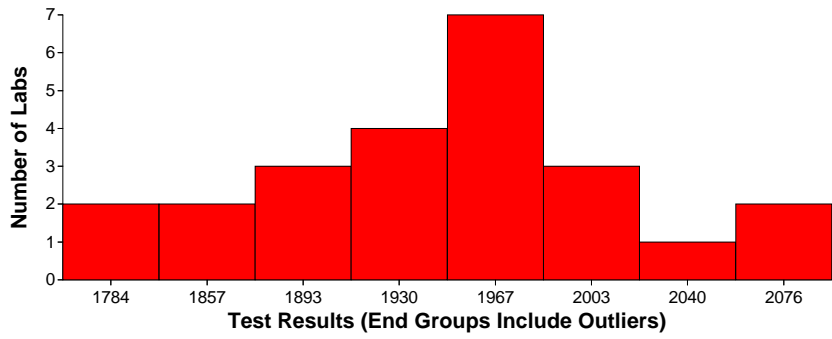

Potable Water Barium, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Barium, Total
 Sample: 0706
 Technology: ICP-MS
 Prep Method:
 Target: 1950 ug/L
 Limits: 1660 to 2240 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 1915.6 ug/L
 Std Dev: 369.75 ug/L
 Median: 1905 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 27 Fail: 1 Total: 28
 Totals for Matrix/Analyte: Labs: Pass: 49 Fail: 3 Total: 52

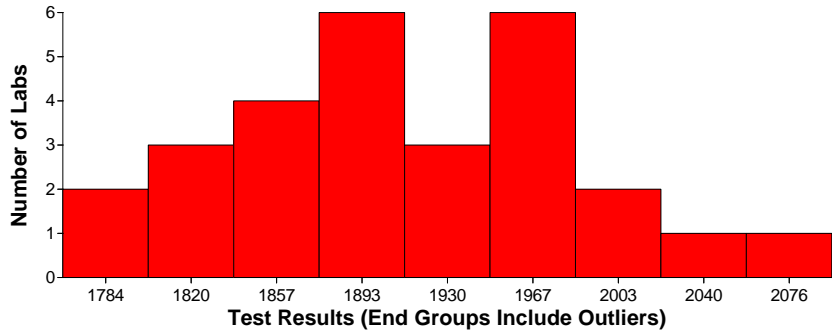

Potable Water Benzo(a)pyrene

Shipment: 407 Matrix: Potable Water
 Analyte: Benzo(a)pyrene
 Sample: 0709
 Technology: GC-MS
 Prep Method:
 Target: 2.22 ug/L
 Limits: 0.944 to 2.81 ug/L
 Basis: Linear Regression
 Robust Mean: 1.9 ug/L
 Std Dev: 0.4681 ug/L
 Median: 1.94 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 13 Fail: 0 Total: 13
 Totals for Matrix/Analyte: Labs: Pass: 13 Fail: 0 Total: 13

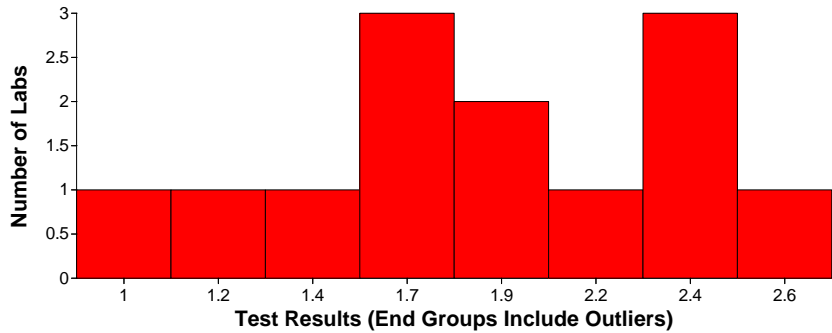

Potable Water Bromobenzene

Shipment: 407 Matrix: Potable Water
 Analyte: Bromobenzene
 Sample: 0721
 Technology: GC-MS
 Prep Method:
 Target: 6.77 ug/L
 Limits: 4.06 to 9.48 ug/L
 Basis: Fixed Percent (2)
 Robust Mean: 6.8 ug/L
 Std Dev: 1.3662 ug/L
 Median: 6.61 ug/L

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 29 Fail: 1 Total: 30
 Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

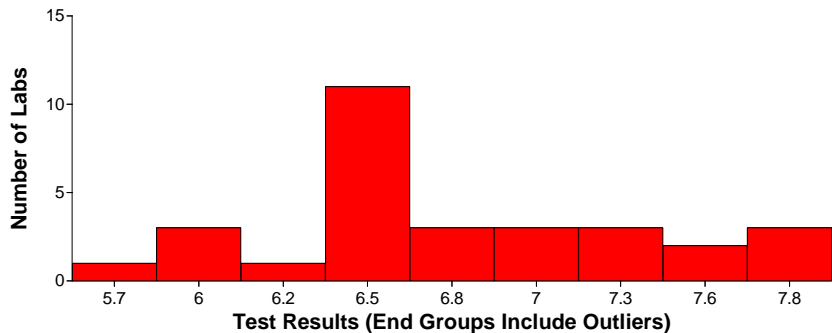

Potable Water Bromobenzene

Shipment: 407 Matrix: Potable Water
Analyte: Bromobenzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 6.77 ug/L
Limits: 4.06 to 9.48 ug/L
Basis: Fixed Percent (2)
Robust Mean: 6.8 ug/L
Std Dev: 0 ug/L
Median: 6.76 ug/L

A histogram is not displayed for
Technology: GCELCD/PID due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water Bromochloroacetic acid

Shipment: 407 Matrix: Potable Water
Analyte: Bromochloroacetic acid
Sample: 0726
Technology: GC-ECD
Prep Method:
Target: 32 ug/L
Limits: 19.2 to 44.8 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 31.8 ug/L
Std Dev: 4.2207 ug/L
Median: 30.25 ug/L

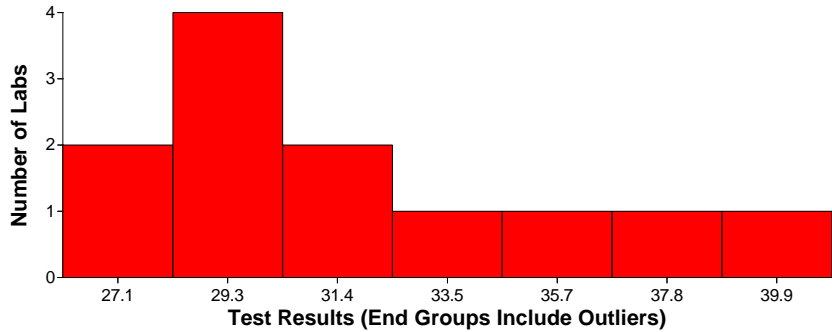


Totals for Matrix/Analyte/Technology:

Labs: Pass: 12 Fail: 0 Total: 12

Totals for Matrix/Analyte: Labs: Pass: 12 Fail: 0 Total: 12

Potable Water Bromochloromethane

Shipment: 407 Matrix: Potable Water
Analyte: Bromochloromethane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 2.29 ug/L
Limits: 1.37 to 3.21 ug/L
Basis: Fixed Percent (2)
Robust Mean: 2.4 ug/L
Std Dev: 0.6352 ug/L
Median: 2.4 ug/L

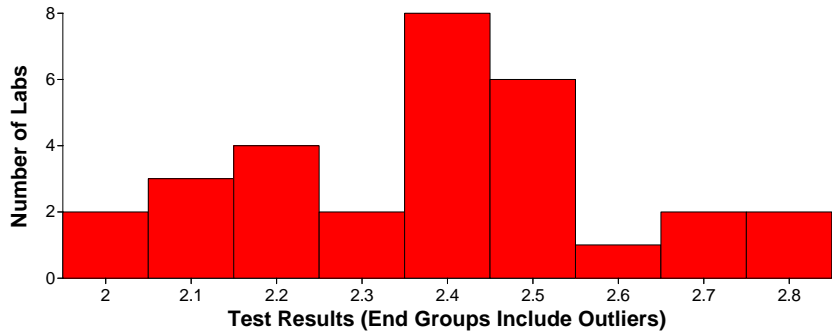

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 2 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water Bromochloromethane

Shipment: 407 Matrix: Potable Water
Analyte: Bromochloromethane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 2.29 ug/L
Limits: 1.37 to 3.21 ug/L
Basis: Fixed Percent (2)
Robust Mean: 2.6 ug/L
Std Dev: 0 ug/L
Median: 2.61 ug/L

A histogram is not displayed for
Technology: GCELCD/PID due to the
limited number of participants.

Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water Beryllium, Total

Potable Water Beryllium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Beryllium, Total
Sample: 0706
Technology: GFAAS
Prep Method:
Target: 12.5 ug/L
Limits: 10.6 to 14.4 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 12 ug/L
Std Dev: 1.4142 ug/L
Median: 12 ug/L

A histogram is not displayed for
Technology: GFAAS due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 2 Fail: 0 Total: 2

Totals for Matrix/Analyte: Labs: Pass: 45 Fail: 5 Total: 50

Potable Water Beryllium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Beryllium, Total
Sample: 0706
Technology: ICP-AES
Prep Method:
Target: 12.5 ug/L
Limits: 10.6 to 14.4 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 12.4 ug/L
Std Dev: 3.9976 ug/L
Median: 12.4 ug/L

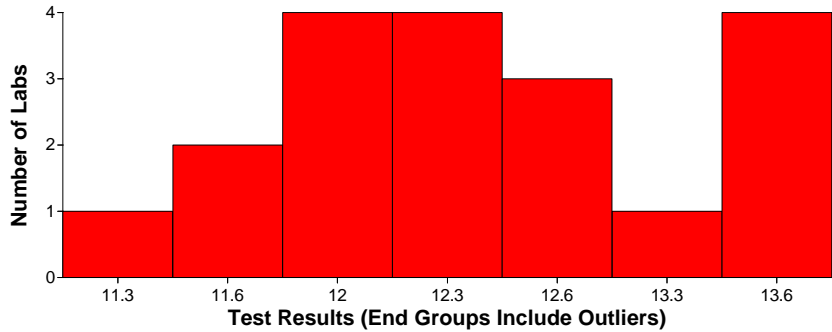


Totals for Matrix/Analyte/Technology:

Labs: Pass: 17 Fail: 2 Total: 19

Totals for Matrix/Analyte: Labs: Pass: 45 Fail: 5 Total: 50

Potable Water Beryllium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Beryllium, Total
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 12.5 ug/L
Limits: 10.6 to 14.4 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 12.4 ug/L
Std Dev: 3.8842 ug/L
Median: 12.4 ug/L

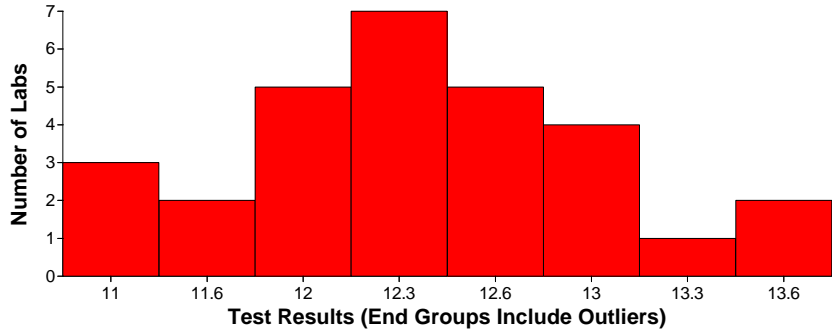


Totals for Matrix/Analyte/Technology:

Labs: Pass: 26 Fail: 3 Total: 29

Totals for Matrix/Analyte: Labs: Pass: 45 Fail: 5 Total: 50

Potable Water Benzene

Shipment: 407 Matrix: Potable Water
Analyte: Benzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 5.1 ug/L
Limits: 3.06 to 7.14 ug/L
Basis: Fixed Percent (2)
Robust Mean: 5.1 ug/L
Std Dev: 0.9991 ug/L
Median: 5.145 ug/L

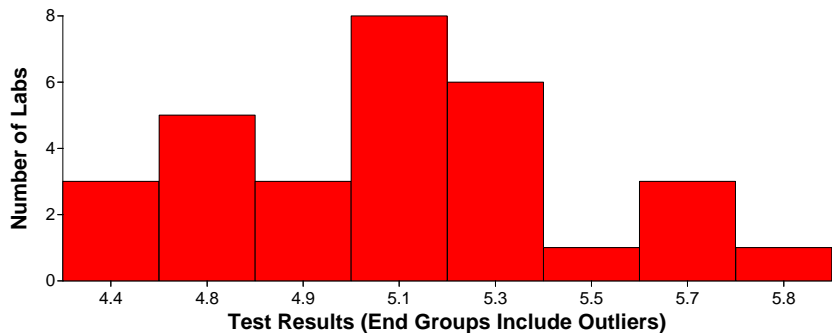

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water Benzene

Shipment: 407 Matrix: Potable Water
Analyte: Benzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 5.1 ug/L
Limits: 3.06 to 7.14 ug/L
Basis: Fixed Percent (2)
Robust Mean: 4.6 ug/L
Std Dev: 0 ug/L
Median: 4.56 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water Bromide

Shipment: 407 Matrix: Potable Water
Analyte: Bromide
Sample: 0729
Technology: IC-COND
Prep Method:
Target: 184 ug/L
Limits: 156 to 212 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 185.7 ug/L
Std Dev: 12.6399 ug/L
Median: 187 ug/L

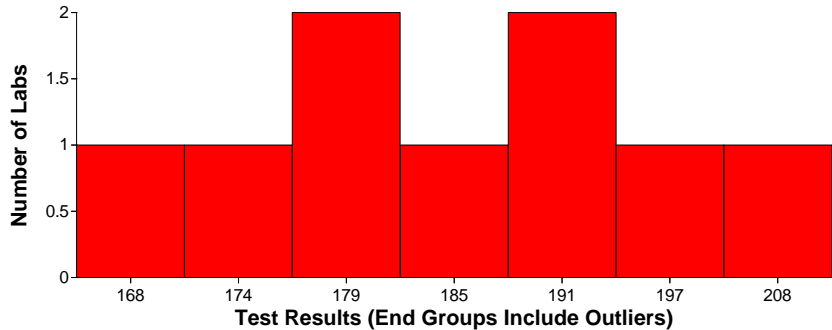


Totals for Matrix/Analyte/Technology:

Labs: Pass: 9 Fail: 0 Total: 9

Totals for Matrix/Analyte: Labs: Pass: 9 Fail: 0 Total: 9

Potable Water Boron, Total

Shipment: 407 Matrix: Potable Water
Analyte: Boron, Total
Sample: 0706
Technology: ICP-AES
Prep Method:
Target: 1050 ug/L
Limits: 893 to 1210 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 1035.4 ug/L
Std Dev: 44.0333 ug/L
Median: 1040 ug/L

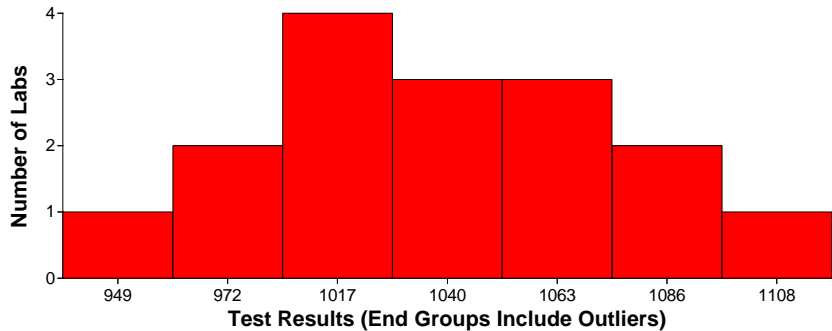


Totals for Matrix/Analyte/Technology:

Labs: Pass: 16 Fail: 0 Total: 16

Totals for Matrix/Analyte: Labs: Pass: 16 Fail: 0 Total: 16

Potable Water Bromodichloromethane

Shipment: 407 Matrix: Potable Water
Analyte: Bromodichloromethane
Sample: 0713
Technology: GC-MS
Prep Method:
Target: 46.5 ug/L
Limits: 37.2 to 55.8 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 47.5 ug/L
Std Dev: 14.0384 ug/L
Median: 48.1 ug/L

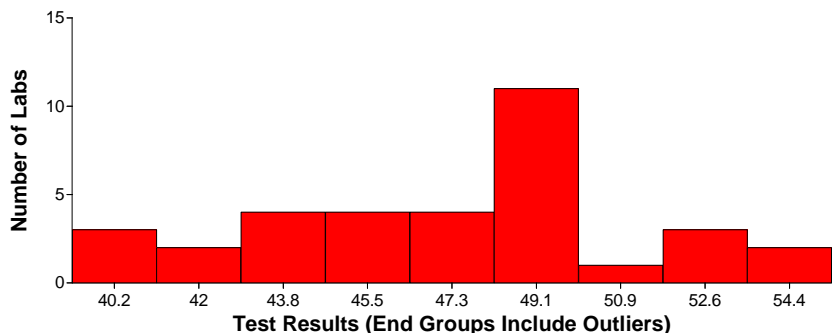

Totals for Matrix/Analyte/Technology:

Labs: Pass: 31 Fail: 3 Total: 34

Totals for Matrix/Analyte: Labs: Pass: 33 Fail: 3 Total: 36

Potable Water Bromodichloromethane

Potable Water Bromodichloromethane

Shipment: 407 Matrix: Potable Water
Analyte: Bromodichloromethane
Sample: 0713
Technology: GCELCD/PID
Prep Method:
Target: 46.5 ug/L
Limits: 37.2 to 55.8 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 45.7 ug/L
Std Dev: 0.4243 ug/L
Median: 45.7 ug/L

A histogram is not displayed for
Technology: GCELCD/PID due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 2 Fail: 0 Total: 2

Totals for Matrix/Analyte: Labs: Pass: 33 Fail: 3 Total: 36

Potable Water Bromoform

Shipment: 407 Matrix: Potable Water
Analyte: Bromoform
Sample: 0713
Technology: GC-MS
Prep Method:
Target: 12.9 ug/L
Limits: 10.3 to 15.5 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 12.7 ug/L
Std Dev: 3.2078 ug/L
Median: 12.55 ug/L

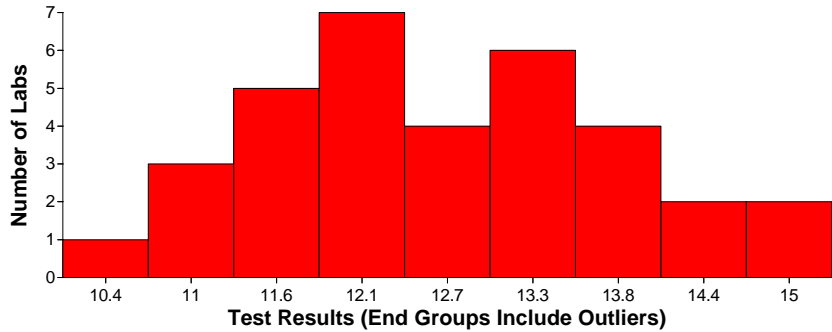

Totals for Matrix/Analyte/Technology:

Labs: Pass: 32 Fail: 2 Total: 34

Totals for Matrix/Analyte: Labs: Pass: 34 Fail: 2 Total: 36

Potable Water Bromoform

Shipment: 407 Matrix: Potable Water
Analyte: Bromoform
Sample: 0713
Technology: GCELCD/PID
Prep Method:
Target: 12.9 ug/L
Limits: 10.3 to 15.5 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 13.5 ug/L
Std Dev: 0.0707 ug/L
Median: 13.45 ug/L

A histogram is not displayed for
Technology: GCELCD/PID due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 2 Fail: 0 Total: 2

Totals for Matrix/Analyte: Labs: Pass: 34 Fail: 2 Total: 36

Potable Water Bromate

Shipment: 407 Matrix: Potable Water
Analyte: Bromate
Sample: 0729
Technology: IC-COND
Prep Method:
Target: 44.3 ug/L
Limits: 31 to 57.6 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 44.6 ug/L
Std Dev: 2.4989 ug/L
Median: 43.7 ug/L

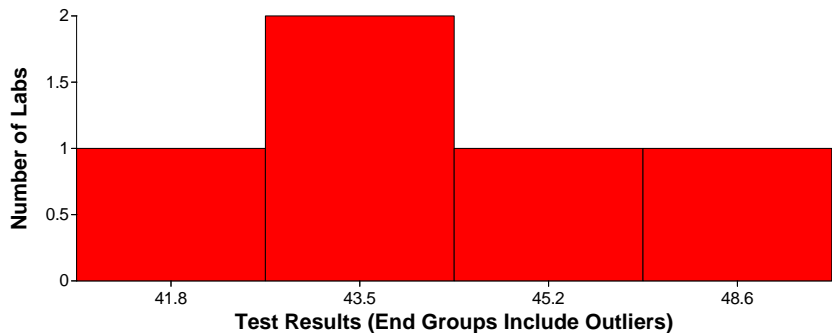

Totals for Matrix/Analyte/Technology:

Labs: Pass: 5 Fail: 0 Total: 5

Totals for Matrix/Analyte: Labs: Pass: 6 Fail: 0 Total: 6

Potable Water Bromate

Shipment: 407 Matrix: Potable Water
Analyte: Bromate
Sample: 0729
Technology: IC-ESI-MS
Prep Method:
Target: 44.3 ug/L
Limits: 31 to 57.6 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 36.9 ug/L
Std Dev: 0 ug/L
Median: 36.9 ug/L

A histogram is not displayed for
Technology: IC-ESI-MS due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 6 Fail: 0 Total: 6

Potable Water Butachlor

Shipment: 407 Matrix: Potable Water
Analyte: Butachlor
Sample: 0707B
Technology: GC-MS
Prep Method:
Target: 9.47 ug/L
Limits: 5.21 to 13.7 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 9.6 ug/L
Std Dev: 1.6833 ug/L
Median: 9.145 ug/L

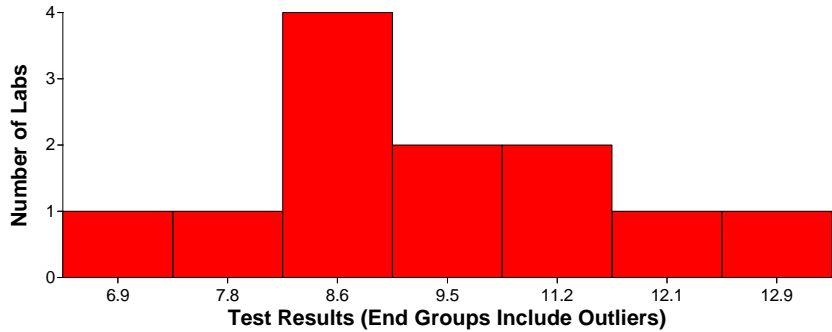


Totals for Matrix/Analyte/Technology:

Labs: Pass: 12 Fail: 0 Total: 12

Totals for Matrix/Analyte: Labs: Pass: 12 Fail: 0 Total: 12

Potable Water Calcium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Calcium, Total
Sample: 0732
Technology: FAAS
Prep Method:
Target: 63.6 mg/L
Limits: 54.1 to 73.1 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 62.7 mg/L
Std Dev: 0.638 mg/L
Median: 63.1 mg/L

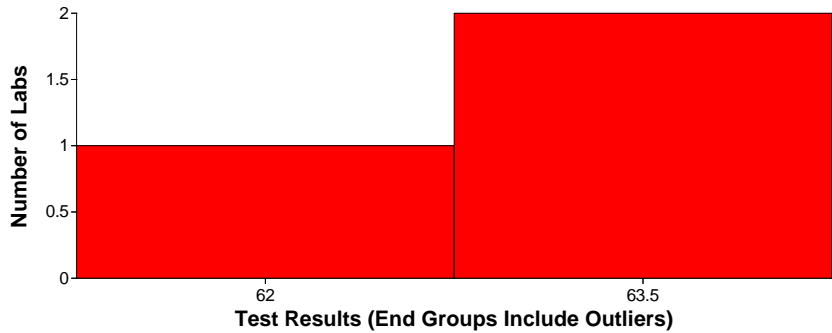

Totals for Matrix/Analyte/Technology:

Labs: Pass: 3 Fail: 0 Total: 3

Totals for Matrix/Analyte: Labs: Pass: 38 Fail: 2 Total: 40

Potable Water Calcium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Calcium, Total
Sample: 0732
Technology: IC
Prep Method:
Target: 63.6 mg/L
Limits: 54.1 to 73.1 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 61 mg/L
Std Dev: 0 mg/L
Median: 61 mg/L

A histogram is not displayed for
Technology: IC due to the limited
number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 38 Fail: 2 Total: 40

Potable Water Calcium, Total

Potable Water Calcium, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Calcium, Total
 Sample: 0732
 Technology: ICP-AES
 Prep Method:
 Target: 63.6 mg/L
 Limits: 54.1 to 73.1 mg/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 63.7 mg/L
 Std Dev: 11.6013 mg/L
 Median: 64.25 mg/L
Totals for Matrix/Analyte/Technology:
 Labs: Pass: 31 Fail: 1 Total: 32
Totals for Matrix/Analyte: Labs: Pass: 38 Fail: 2 Total: 40

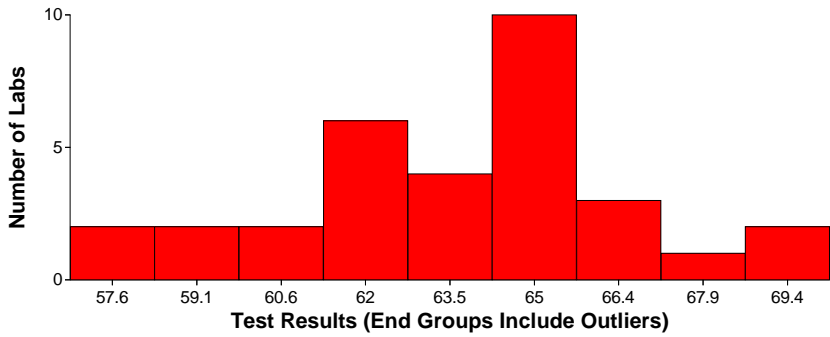


Potable Water Calcium, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Calcium, Total
 Sample: 0732
 Technology: ICP-MS
 Prep Method:
 Target: 63.6 mg/L
 Limits: 54.1 to 73.1 mg/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 69.5 mg/L
 Std Dev: 0 mg/L
 Median: 69.5 mg/L
Totals for Matrix/Analyte/Technology:
 Labs: Pass: 1 Fail: 0 Total: 1
Totals for Matrix/Analyte: Labs: Pass: 38 Fail: 2 Total: 40

A histogram is not displayed for Technology: ICP-MS due to the limited number of participants.


Potable Water Calcium, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Calcium, Total
 Sample: 0732
 Technology: TITR
 Prep Method:
 Target: 63.6 mg/L
 Limits: 54.1 to 73.1 mg/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 60.8 mg/L
 Std Dev: 35.0929 mg/L
 Median: 61.9 mg/L
Totals for Matrix/Analyte/Technology:
 Labs: Pass: 2 Fail: 1 Total: 3
Totals for Matrix/Analyte: Labs: Pass: 38 Fail: 2 Total: 40

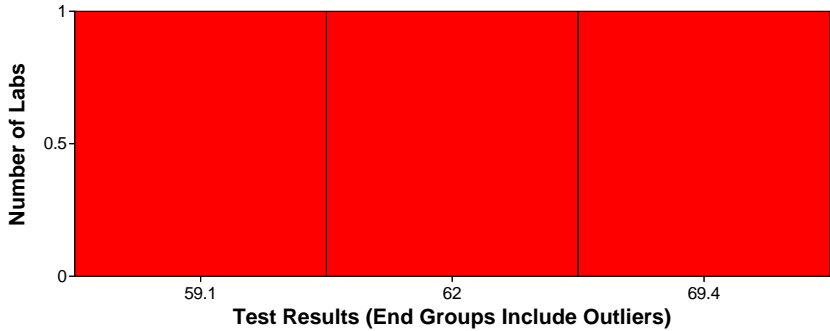

Potable Water Carbofuran


Shipment: 407 Matrix: Potable Water
 Analyte: Carbofuran
 Sample: 0715
 Technology: HPLC-FLUOR
 Prep Method:
 Target: 31 ug/L
 Limits: 17.1 to 45 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 29.9 ug/L
 Std Dev: 1.7374 ug/L
 Median: 30.5 ug/L
Totals for Matrix/Analyte/Technology:
 Labs: Pass: 9 Fail: 0 Total: 9
Totals for Matrix/Analyte: Labs: Pass: 9 Fail: 0 Total: 9

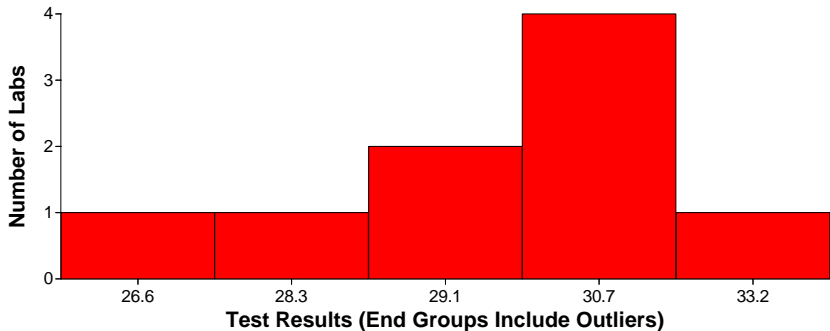

Potable Water Carbaryl


Potable Water Carbaryl

Shipment: 407 Matrix: Potable Water
Analyte: Carbaryl
Sample: 0715
Technology: HPLC-FLUOR
Prep Method:
Target: 50 ug/L
Limits: 37.5 to 62.5 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 48.9 ug/L
Std Dev: 16.3555 ug/L
Median: 48.2 ug/L
Totals for Matrix/Analyte/Technology:
Labs: Pass: 9 Fail: 0 Total: 9
Totals for Matrix/Analyte: Labs: Pass: 9 Fail: 0 Total: 9

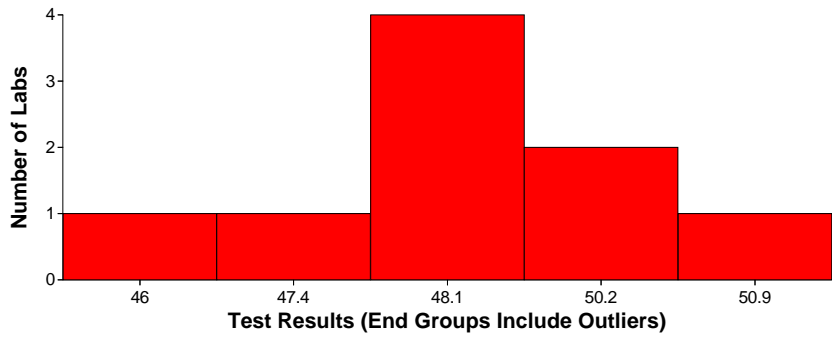

Potable Water Carbon tetrachloride

Shipment: 407 Matrix: Potable Water
Analyte: Carbon tetrachloride
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 6.42 ug/L
Limits: 3.85 to 8.99 ug/L
Basis: Fixed Percent (2)
Robust Mean: 6.4 ug/L
Std Dev: 1.46 ug/L
Median: 6.405 ug/L
Totals for Matrix/Analyte/Technology:
Labs: Pass: 29 Fail: 1 Total: 30
Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

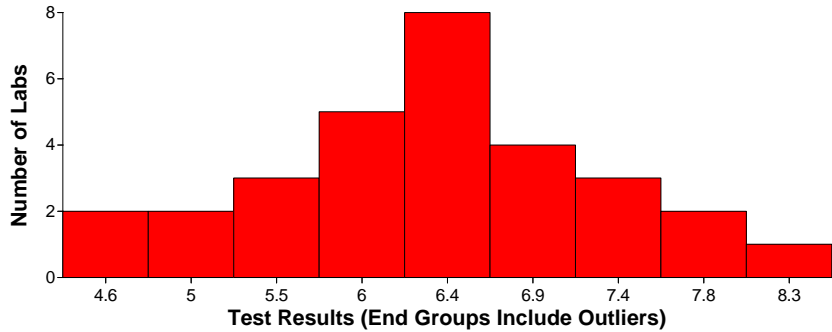


Potable Water Carbon tetrachloride

Shipment: 407 Matrix: Potable Water
Analyte: Carbon tetrachloride
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 6.42 ug/L
Limits: 3.85 to 8.99 ug/L
Basis: Fixed Percent (2)
Robust Mean: 7 ug/L
Std Dev: 0 ug/L
Median: 7.04 ug/L
Totals for Matrix/Analyte/Technology:
Labs: Pass: 1 Fail: 0 Total: 1
Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Potable Water Cadmium, Total


Shipment: 407 Matrix: Potable Water
Analyte: Cadmium, Total
Sample: 0706
Technology: GFAAS
Prep Method:
Target: 7.48 ug/L
Limits: 5.98 to 8.98 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 7.7 ug/L
Std Dev: 0.4302 ug/L
Median: 7.65 ug/L
Totals for Matrix/Analyte/Technology:
Labs: Pass: 3 Fail: 0 Total: 3
Totals for Matrix/Analyte: Labs: Pass: 50 Fail: 3 Total: 53

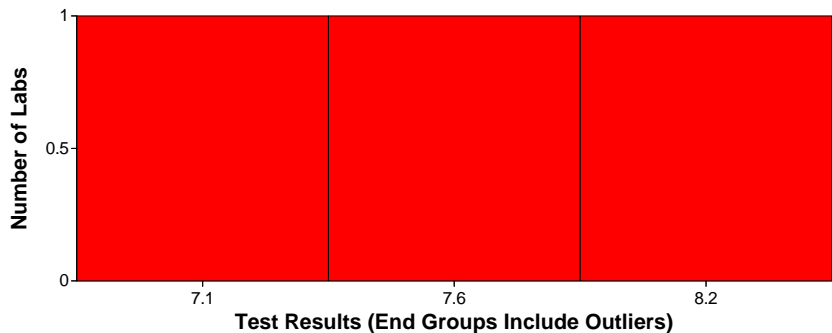

Potable Water Cadmium, Total

Potable Water Cadmium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Cadmium, Total
Sample: 0706
Technology: ICP-AES
Prep Method:
Target: 7.48 ug/L
Limits: 5.98 to 8.98 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 7.8 ug/L
Std Dev: 2.3826 ug/L
Median: 7.8 ug/L

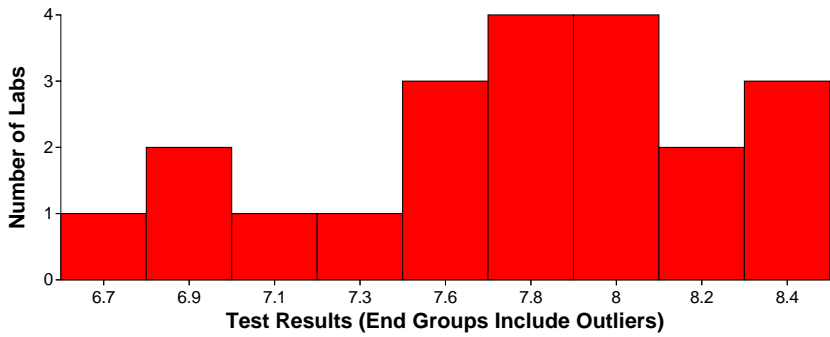


Totals for Matrix/Analyte/Technology:

Labs: Pass: 19 Fail: 2 Total: 21

Totals for Matrix/Analyte: Labs: Pass: 50 Fail: 3 Total: 53

Potable Water Cadmium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Cadmium, Total
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 7.48 ug/L
Limits: 5.98 to 8.98 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 7.4 ug/L
Std Dev: 1.435 ug/L
Median: 7.44 ug/L

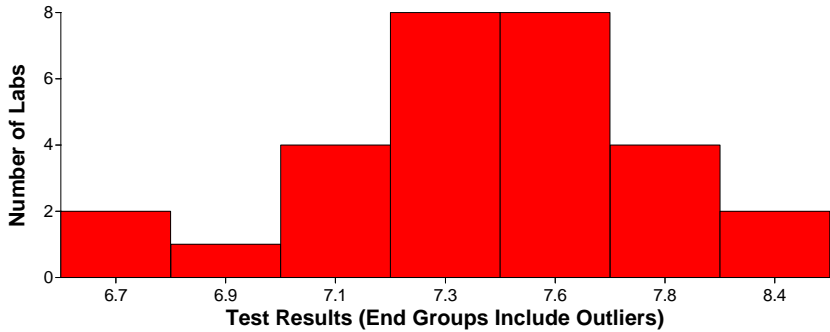


Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 1 Total: 29

Totals for Matrix/Analyte: Labs: Pass: 50 Fail: 3 Total: 53

Potable Water Bromomethane

Shipment: 407 Matrix: Potable Water
Analyte: Bromomethane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 31.2 ug/L
Limits: 18.7 to 43.7 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 30.3 ug/L
Std Dev: 5.6867 ug/L
Median: 30.25 ug/L

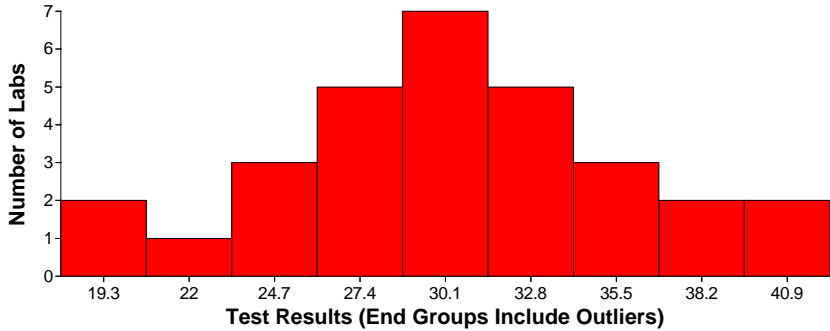

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water Bromomethane

Shipment: 407 Matrix: Potable Water
Analyte: Bromomethane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 31.2 ug/L
Limits: 18.7 to 43.7 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 25.7 ug/L
Std Dev: 0 ug/L
Median: 25.7 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water Chloromethane

Potable Water Chloromethane

Shipment: 407 Matrix: Potable Water
Analyte: Chloromethane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 24.9 ug/L
Limits: 14.9 to 34.9 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 27 ug/L
Std Dev: 3.9414 ug/L
Median: 26.9 ug/L

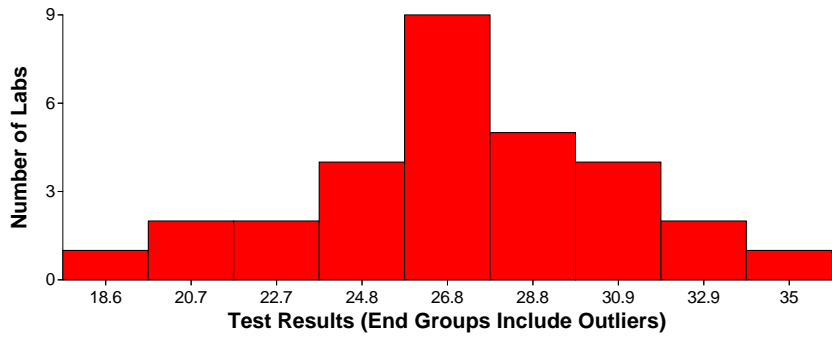

Totals for Matrix/Analyte/Technology:
Labs: Pass: 30 Fail: 0 Total: 30
Totals for Matrix/Analyte: Labs: Pass: 31 Fail: 0 Total: 31

Potable Water Chloromethane

Shipment: 407 Matrix: Potable Water
Analyte: Chloromethane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 24.9 ug/L
Limits: 14.9 to 34.9 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 21.1 ug/L
Std Dev: 0 ug/L
Median: 21.1 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
Labs: Pass: 1 Fail: 0 Total: 1
Totals for Matrix/Analyte: Labs: Pass: 31 Fail: 0 Total: 31

Potable Water Calcium Hardness


Shipment: 407 Matrix: Potable Water
Analyte: Calcium Hardness
Sample: 0703
Technology: AUTO
Prep Method:
Target: 80.5 mg/L
Limits: 68.4 to 92.6 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 81.8 mg/L
Std Dev: 0 mg/L
Median: 81.8 mg/L

A histogram is not displayed for Technology: AUTO due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
Labs: Pass: 1 Fail: 0 Total: 1
Totals for Matrix/Analyte: Labs: Pass: 47 Fail: 1 Total: 48

Potable Water Calcium Hardness

Shipment: 407 Matrix: Potable Water
Analyte: Calcium Hardness
Sample: 0703
Technology: CALC
Prep Method:
Target: 80.5 mg/L
Limits: 68.4 to 92.6 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 80.1 mg/L
Std Dev: 3.0956 mg/L
Median: 78.9 mg/L

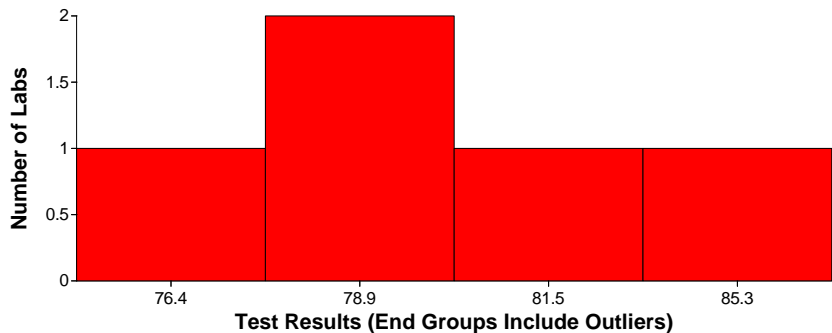

Totals for Matrix/Analyte/Technology:
Labs: Pass: 5 Fail: 0 Total: 5
Totals for Matrix/Analyte: Labs: Pass: 47 Fail: 1 Total: 48

Potable Water Calcium Hardness

Shipment: 407 Matrix: Potable Water
Analyte: Calcium Hardness
Sample: 0703
Technology: FAAS
Prep Method:
Target: 80.5 mg/L
Limits: 68.4 to 92.6 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 81.5 mg/L
Std Dev: 0 mg/L
Median: 81.5 mg/L

A histogram is not displayed for
Technology: FAAS due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 47 Fail: 1 Total: 48

Potable Water Calcium Hardness

Shipment: 407 Matrix: Potable Water
Analyte: Calcium Hardness
Sample: 0703
Technology: ICP-AES
Prep Method:
Target: 80.5 mg/L
Limits: 68.4 to 92.6 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 80.6 mg/L
Std Dev: 22.9138 mg/L
Median: 80.7 mg/L

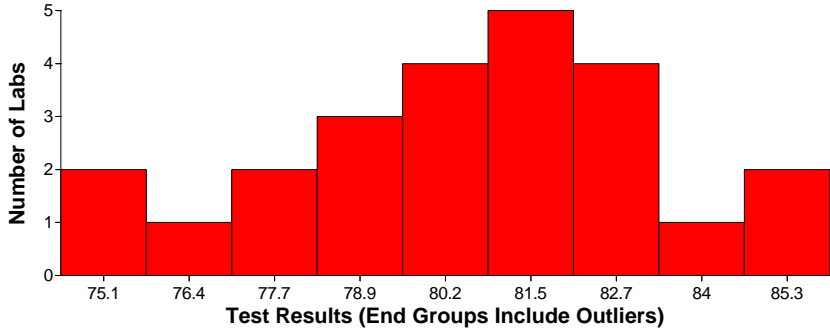


Totals for Matrix/Analyte/Technology:

Labs: Pass: 23 Fail: 1 Total: 24

Totals for Matrix/Analyte: Labs: Pass: 47 Fail: 1 Total: 48

Potable Water Calcium Hardness

Shipment: 407 Matrix: Potable Water
Analyte: Calcium Hardness
Sample: 0703
Technology: TITR
Prep Method:
Target: 80.5 mg/L
Limits: 68.4 to 92.6 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 79.3 mg/L
Std Dev: 2.1689 mg/L
Median: 79.8 mg/L

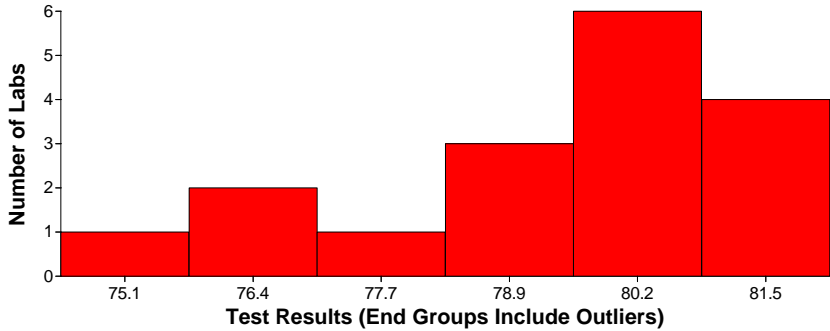

Totals for Matrix/Analyte/Technology:

Labs: Pass: 17 Fail: 0 Total: 17

Totals for Matrix/Analyte: Labs: Pass: 47 Fail: 1 Total: 48

Potable Water Chloride

Shipment: 407 Matrix: Potable Water
Analyte: Chloride
Sample: 0702
Technology: AUTO
Prep Method:
Target: 144 mg/L
Limits: 122 to 166 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 149 mg/L
Std Dev: 0 mg/L
Median: 149 mg/L

A histogram is not displayed for
Technology: AUTO due to the
limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 58 Fail: 2 Total: 60

Potable Water Chloride

Potable Water Chloride

Shipment: 407 Matrix: Potable Water
Analyte: Chloride
Sample: 0702
Technology: COLOR
Prep Method:
Target: 144 mg/L
Limits: 122 to 166 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 143.2 mg/L
Std Dev: 5.5648 mg/L
Median: 144.5 mg/L

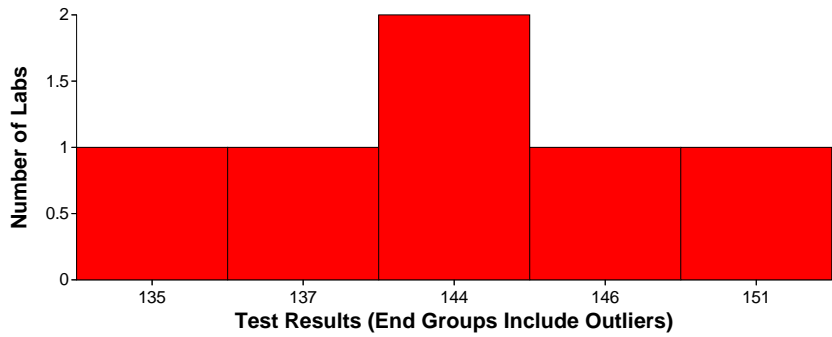


Totals for Matrix/Analyte/Technology:

Labs: Pass: 6 Fail: 0 Total: 6

Totals for Matrix/Analyte: Labs: Pass: 58 Fail: 2 Total: 60

Potable Water Chloride

Shipment: 407 Matrix: Potable Water
Analyte: Chloride
Sample: 0702
Technology: IC-COND
Prep Method:
Target: 144 mg/L
Limits: 122 to 166 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 143.2 mg/L
Std Dev: 41.4906 mg/L
Median: 144 mg/L

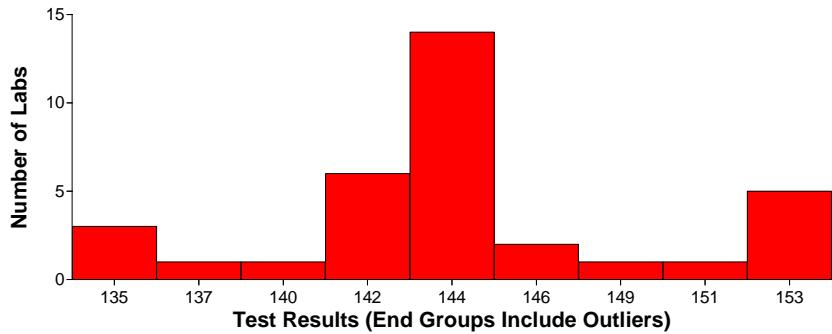


Totals for Matrix/Analyte/Technology:

Labs: Pass: 32 Fail: 2 Total: 34

Totals for Matrix/Analyte: Labs: Pass: 58 Fail: 2 Total: 60

Potable Water Chloride

Shipment: 407 Matrix: Potable Water
Analyte: Chloride
Sample: 0702
Technology: TITR
Prep Method:
Target: 144 mg/L
Limits: 122 to 166 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 145.2 mg/L
Std Dev: 3.9081 mg/L
Median: 145 mg/L

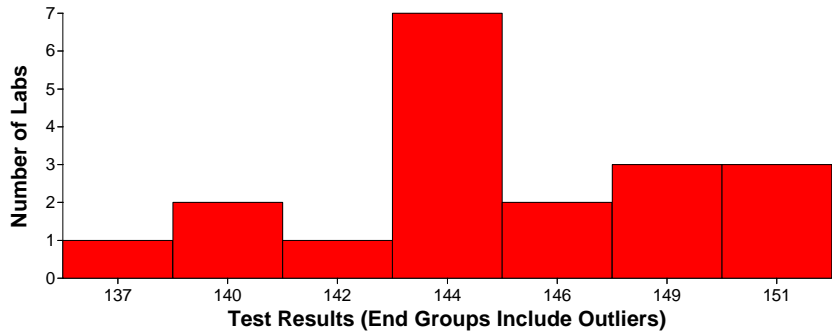


Totals for Matrix/Analyte/Technology:

Labs: Pass: 19 Fail: 0 Total: 19

Totals for Matrix/Analyte: Labs: Pass: 58 Fail: 2 Total: 60

Potable Water Chlordane Total

Shipment: 407 Matrix: Potable Water
Analyte: Chlordane Total
Sample: 0714
Technology: GC-ECD
Prep Method:
Target: 7.12 ug/L
Limits: 3.92 to 10.3 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 6.6 ug/L
Std Dev: 0.7934 ug/L
Median: 6.42 ug/L

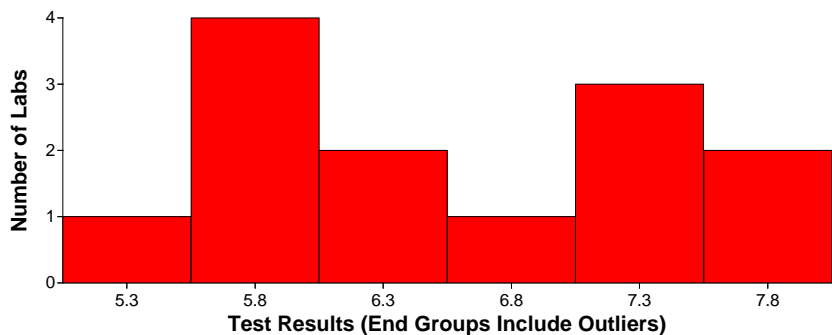

Totals for Matrix/Analyte/Technology:


Labs: Pass: 13 Fail: 0 Total: 13

Totals for Matrix/Analyte: Labs: Pass: 16 Fail: 0 Total: 16

Potable Water Chlordane Total

Potable Water Chlordane Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Chlordane Total
Sample: 0714
Technology: GC-MS
Prep Method:
Target: 7.12 ug/L
Limits: 3.92 to 10.3 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 5.2 ug/L
Std Dev: 0.852 ug/L
Median: 5.1 ug/L

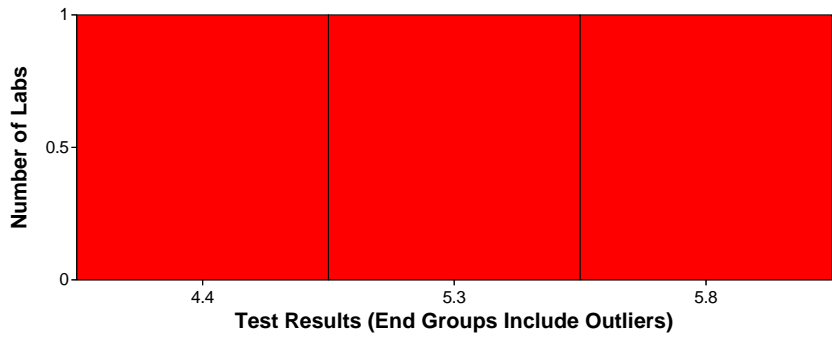


Totals for Matrix/Analyte/Technology:
Labs: Pass: 3 **Fail:** 0 **Total:** 3

Totals for Matrix/Analyte: **Labs: Pass:** 16 **Fail:** 0 **Total:** 16

Potable Water Chlorobenzene

Shipment: 407 **Matrix:** Potable Water
Analyte: Chlorobenzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 2.24 ug/L
Limits: 1.34 to 3.14 ug/L
Basis: Fixed Percent (2)
Robust Mean: 2.2 ug/L
Std Dev: 0.5882 ug/L
Median: 2.195 ug/L

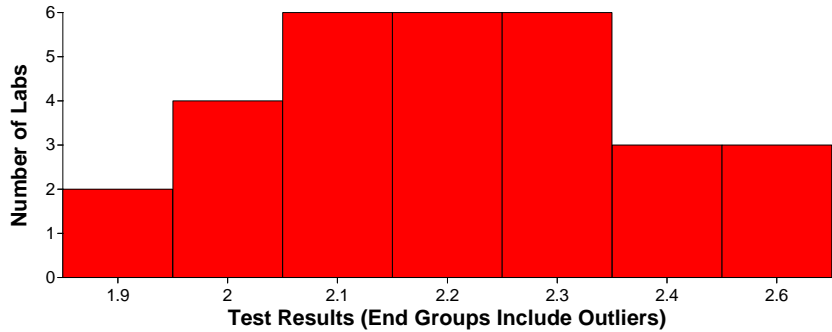

Totals for Matrix/Analyte/Technology:
Labs: Pass: 29 **Fail:** 1 **Total:** 30

Totals for Matrix/Analyte: **Labs: Pass:** 30 **Fail:** 1 **Total:** 31

Potable Water Chlorobenzene

Shipment: 407 **Matrix:** Potable Water
Analyte: Chlorobenzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 2.24 ug/L
Limits: 1.34 to 3.14 ug/L
Basis: Fixed Percent (2)
Robust Mean: 2.3 ug/L
Std Dev: 0 ug/L
Median: 2.27 ug/L


A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
Labs: Pass: 1 **Fail:** 0 **Total:** 1

Totals for Matrix/Analyte: **Labs: Pass:** 30 **Fail:** 1 **Total:** 31

Potable Water Dibromochloromethane

Shipment: 407 **Matrix:** Potable Water
Analyte: Dibromochloromethane
Sample: 0713
Technology: GC-MS
Prep Method:
Target: 49 ug/L
Limits: 39.2 to 58.8 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 49.3 ug/L
Std Dev: 14.5296 ug/L
Median: 48.5 ug/L

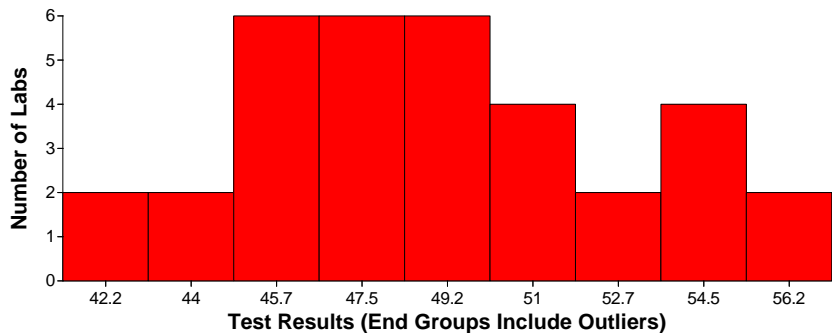

Totals for Matrix/Analyte/Technology:
Labs: Pass: 31 **Fail:** 3 **Total:** 34

Totals for Matrix/Analyte: **Labs: Pass:** 33 **Fail:** 3 **Total:** 36

Potable Water Dibromochloromethane

Potable Water Dibromochloromethane

Shipment: 407 Matrix: Potable Water
Analyte: Dibromochloromethane
Sample: 0713
Technology: GCELCD/PID
Prep Method:
Target: 49 ug/L
Limits: 39.2 to 58.8 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 51.1 ug/L
Std Dev: 2.8991 ug/L
Median: 51.05 ug/L

A histogram is not displayed for
Technology: GCELCD/PID due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 2 Fail: 0 Total: 2

Totals for Matrix/Analyte: Labs: Pass: 33 Fail: 3 Total: 36

Potable Water Chloroethane

Shipment: 407 Matrix: Potable Water
Analyte: Chloroethane
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 46 ug/L
Limits: 27.6 to 64.4 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 47.4 ug/L
Std Dev: 10.3247 ug/L
Median: 46.3 ug/L

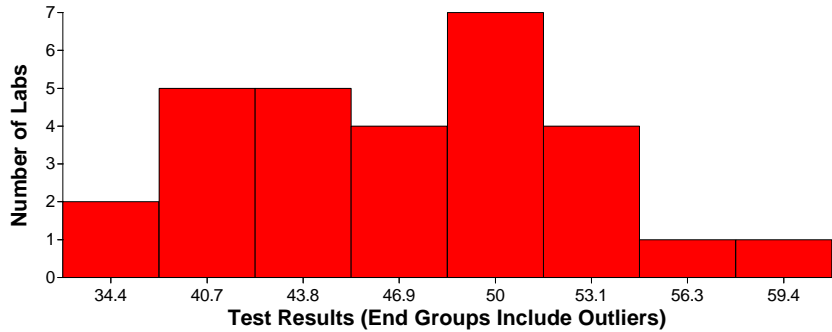

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 1 Total: 29

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 1 Total: 30

Potable Water Chloroethane

Shipment: 407 Matrix: Potable Water
Analyte: Chloroethane
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 46 ug/L
Limits: 27.6 to 64.4 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 35.8 ug/L
Std Dev: 0 ug/L
Median: 35.8 ug/L

A histogram is not displayed for
Technology: GCELCD/PID due to the
limited number of participants.

Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 1 Total: 30

Potable Water Chlorite

Shipment: 407 Matrix: Potable Water
Analyte: Chlorite
Sample: 0730
Technology: AMP
Prep Method:
Target: 102 ug/L
Limits: 71.4 to 133 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 85.6 ug/L
Std Dev: 0 ug/L
Median: 85.6 ug/L

A histogram is not displayed for
Technology: AMP due to the
limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 5 Fail: 2 Total: 7

Potable Water Chlorite

Potable Water Chlorite


Shipment: 407 **Matrix:** Potable Water
Analyte: Chlorite
Sample: 0730
Technology: IC-COND
Prep Method:
Target: 102 ug/L
Limits: 71.4 to 133 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 103.4 ug/L
Std Dev: 53.6142 ug/L
Median: 108.5 ug/L

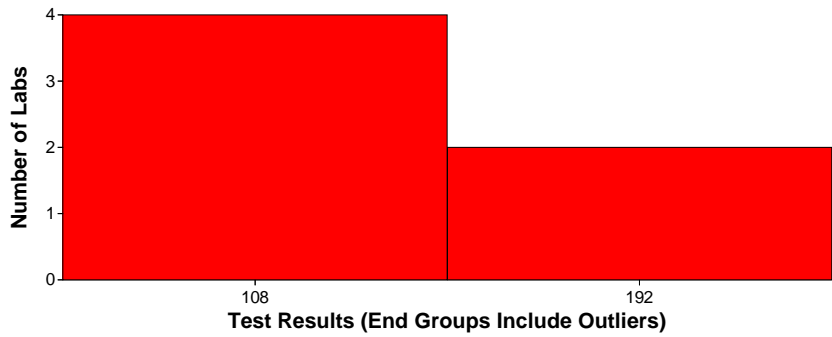

Totals for Matrix/Analyte/Technology:
Labs: Pass: 4 **Fail:** 2 **Total:** 6
Totals for Matrix/Analyte: **Labs: Pass:** 5 **Fail:** 2 **Total:** 7

Potable Water Chlorate


Shipment: 407 **Matrix:** Potable Water
Analyte: Chlorate
Sample: 0730
Technology: IC-COND
Prep Method:
Target: 84.2 ug/L
Limits: 58.9 to 109 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 81.6 ug/L
Std Dev: 6.0095 ug/L
Median: 81.65 ug/L

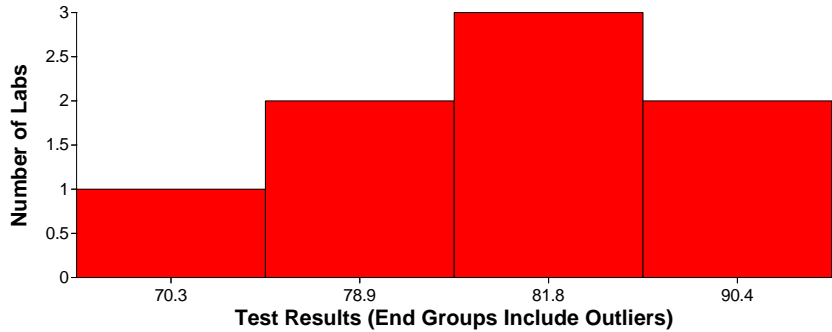

Totals for Matrix/Analyte/Technology:
Labs: Pass: 8 **Fail:** 0 **Total:** 8
Totals for Matrix/Analyte: **Labs: Pass:** 8 **Fail:** 0 **Total:** 8

Potable Water Chloroform

Shipment: 407 **Matrix:** Potable Water
Analyte: Chloroform
Sample: 0713
Technology: GC-MS
Prep Method:
Target: 17.4 ug/L
Limits: 13.9 to 20.9 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 18 ug/L
Std Dev: 3.386 ug/L
Median: 18 ug/L

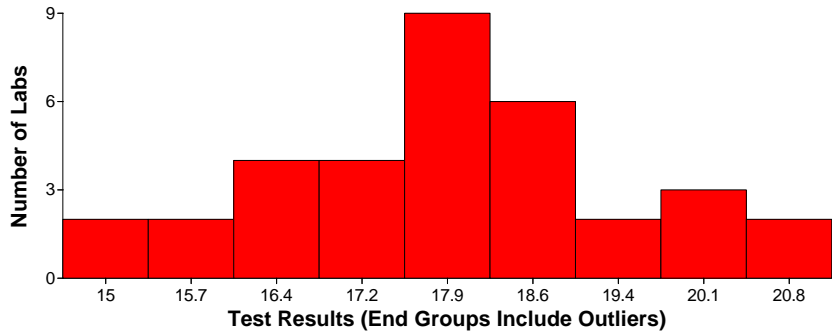

Totals for Matrix/Analyte/Technology:
Labs: Pass: 33 **Fail:** 1 **Total:** 34
Totals for Matrix/Analyte: **Labs: Pass:** 35 **Fail:** 1 **Total:** 36

Potable Water Chloroform

Shipment: 407 **Matrix:** Potable Water
Analyte: Chloroform
Sample: 0713
Technology: GCELCD/PID
Prep Method:
Target: 17.4 ug/L
Limits: 13.9 to 20.9 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 16.3 ug/L
Std Dev: 1.5556 ug/L
Median: 16.3 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
Labs: Pass: 2 **Fail:** 0 **Total:** 2
Totals for Matrix/Analyte: **Labs: Pass:** 35 **Fail:** 1 **Total:** 36

Potable Water Cyanide

Shipment: 407 Matrix: Potable Water
Analyte: Cyanide
Sample: 0705
Technology: AMP
Prep Method:
Target: 0.432 mg/L
Limits: 0.324 to 0.54 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 0.4 mg/L
Std Dev: 0 mg/L
Median: 0.39 mg/L

A histogram is not displayed for
Technology: AMP due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 25 Fail: 1 Total: 26

Potable Water Cyanide

Shipment: 407 Matrix: Potable Water
Analyte: Cyanide
Sample: 0705
Technology: AUTO
Prep Method:
Target: 0.432 mg/L
Limits: 0.324 to 0.54 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 0.4 mg/L
Std Dev: 0.1201 mg/L
Median: 0.41 mg/L

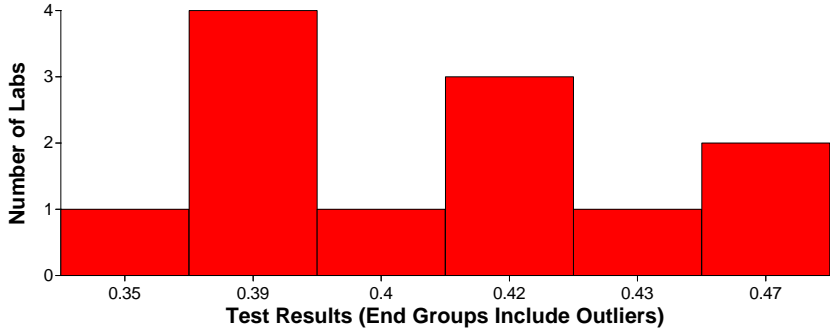


Totals for Matrix/Analyte/Technology:

Labs: Pass: 12 Fail: 0 Total: 12

Totals for Matrix/Analyte: Labs: Pass: 25 Fail: 1 Total: 26

Potable Water Cyanide

Shipment: 407 Matrix: Potable Water
Analyte: Cyanide
Sample: 0705
Technology: COLOR
Prep Method:
Target: 0.432 mg/L
Limits: 0.324 to 0.54 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 0.4 mg/L
Std Dev: 0.1203 mg/L
Median: 0.4 mg/L

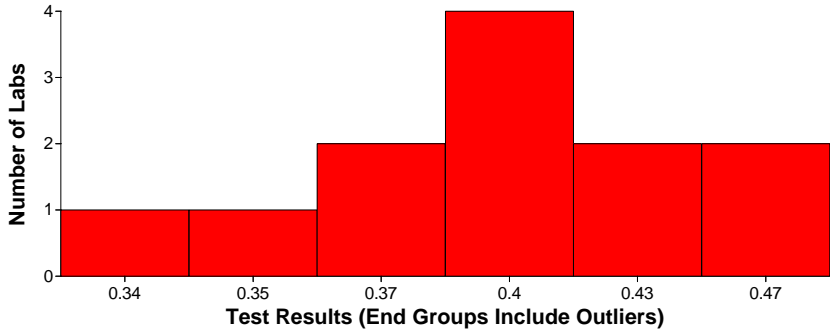

Totals for Matrix/Analyte/Technology:

Labs: Pass: 11 Fail: 1 Total: 12

Totals for Matrix/Analyte: Labs: Pass: 25 Fail: 1 Total: 26

Potable Water Cyanide

Shipment: 407 Matrix: Potable Water
Analyte: Cyanide
Sample: 0705
Technology: POT
Prep Method:
Target: 0.432 mg/L
Limits: 0.324 to 0.54 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 0.4 mg/L
Std Dev: 0 mg/L
Median: 0.41 mg/L

A histogram is not displayed for
Technology: POT due to the
limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 25 Fail: 1 Total: 26

Potable Water Corrosivity


Potable Water Corrosivity

Shipment: 407 **Matrix:** Potable Water
Analyte: Corrosivity
Sample: 0738
Technology: CALC
Prep Method:
Target: 1.19 Saturation Index
Limits: 0.79 to 1.59 Saturation Index
Basis: PW Corrosivity
Robust Mean: 1.2 Saturation Index
Std Dev: 0.3296 Saturation Index
Median: 1.225 Saturation Index
Totals for Matrix/Analyte/Technology:
Labs: Pass: 15 **Fail:** 1 **Total:** 16
Totals for Matrix/Analyte: **Labs: Pass:** 15 **Fail:** 1 **Total:** 16

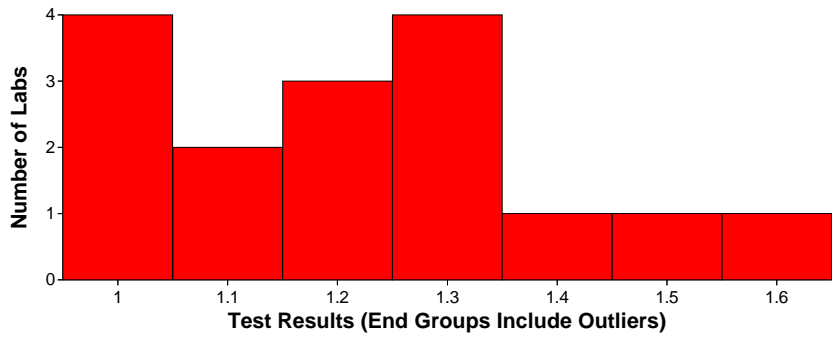


Potable Water Chromium, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Chromium, Total
Sample: 0706
Technology: GFAAS
Prep Method:
Target: 72.4 ug/L
Limits: 61.5 to 83.3 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 73.2 ug/L
Std Dev: 2.94 ug/L
Median: 72.4 ug/L
Totals for Matrix/Analyte/Technology:
Labs: Pass: 3 **Fail:** 0 **Total:** 3
Totals for Matrix/Analyte: **Labs: Pass:** 51 **Fail:** 3 **Total:** 54

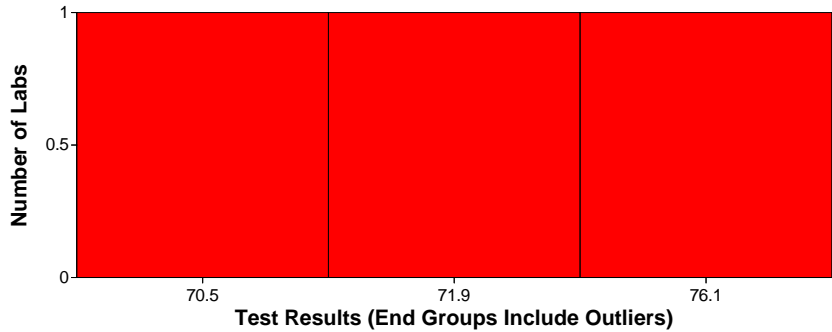


Potable Water Chromium, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Chromium, Total
Sample: 0706
Technology: ICP-AES
Prep Method:
Target: 72.4 ug/L
Limits: 61.5 to 83.3 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 72 ug/L
Std Dev: 15.5841 ug/L
Median: 72.25 ug/L
Totals for Matrix/Analyte/Technology:
Labs: Pass: 21 **Fail:** 1 **Total:** 22
Totals for Matrix/Analyte: **Labs: Pass:** 51 **Fail:** 3 **Total:** 54

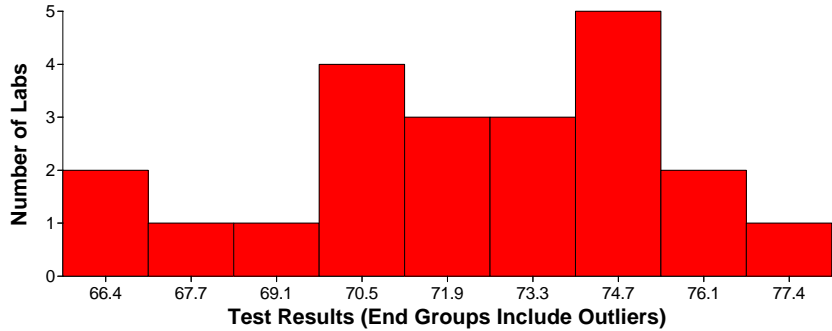

Potable Water Chromium, Total


Shipment: 407 **Matrix:** Potable Water
Analyte: Chromium, Total
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 72.4 ug/L
Limits: 61.5 to 83.3 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 71.3 ug/L
Std Dev: 22.2164 ug/L
Median: 72 ug/L
Totals for Matrix/Analyte/Technology:
Labs: Pass: 27 **Fail:** 2 **Total:** 29
Totals for Matrix/Analyte: **Labs: Pass:** 51 **Fail:** 3 **Total:** 54

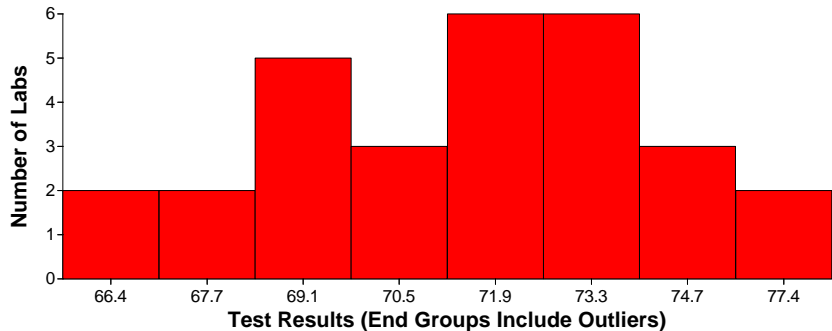

Potable Water Copper, Total

Potable Water Copper, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Copper, Total
 Sample: 0706
 Technology: FAAS
 Prep Method:
 Target: 952 ug/L
 Limits: 857 to 1050 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 927 ug/L
 Std Dev: 35.2177 ug/L
 Median: 928.5 ug/L

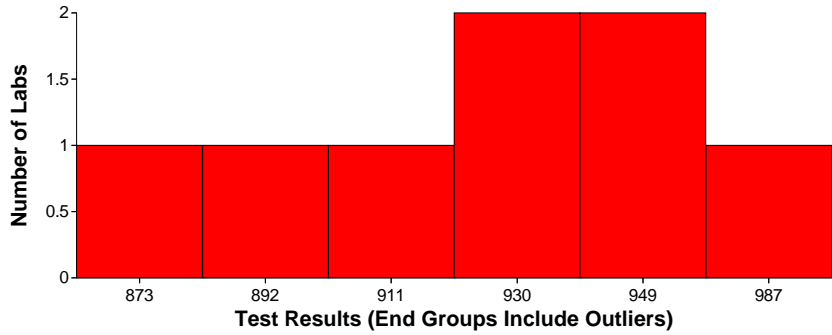

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 8 Fail: 0 Total: 8
 Totals for Matrix/Analyte: Labs: Pass: 63 Fail: 4 Total: 67

Potable Water Copper, Total


Shipment: 407 Matrix: Potable Water
 Analyte: Copper, Total
 Sample: 0706
 Technology: GFAAS
 Prep Method:
 Target: 952 ug/L
 Limits: 857 to 1050 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 949 ug/L
 Std Dev: 0 ug/L
 Median: 949 ug/L

A histogram is not displayed for Technology: GFAAS due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 1 Fail: 0 Total: 1
 Totals for Matrix/Analyte: Labs: Pass: 63 Fail: 4 Total: 67

Potable Water Copper, Total


Shipment: 407 Matrix: Potable Water
 Analyte: Copper, Total
 Sample: 0706
 Technology: ICP-AES
 Prep Method:
 Target: 952 ug/L
 Limits: 857 to 1050 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 950.8 ug/L
 Std Dev: 306.33 ug/L
 Median: 958 ug/L

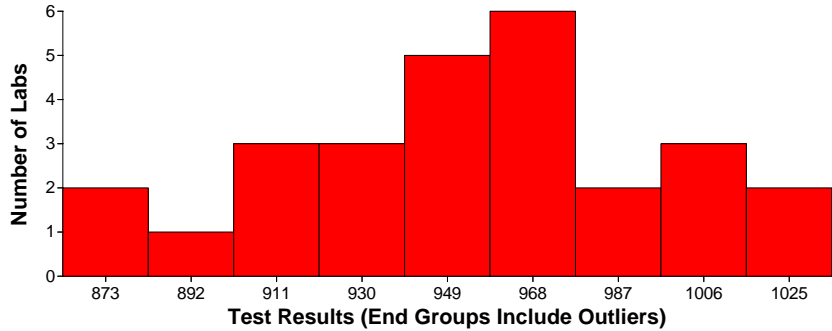

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 24 Fail: 3 Total: 27
 Totals for Matrix/Analyte: Labs: Pass: 63 Fail: 4 Total: 67

Potable Water Copper, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Copper, Total
 Sample: 0706
 Technology: ICP-MS
 Prep Method:
 Target: 952 ug/L
 Limits: 857 to 1050 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 952.1 ug/L
 Std Dev: 175.679 ug/L
 Median: 949 ug/L

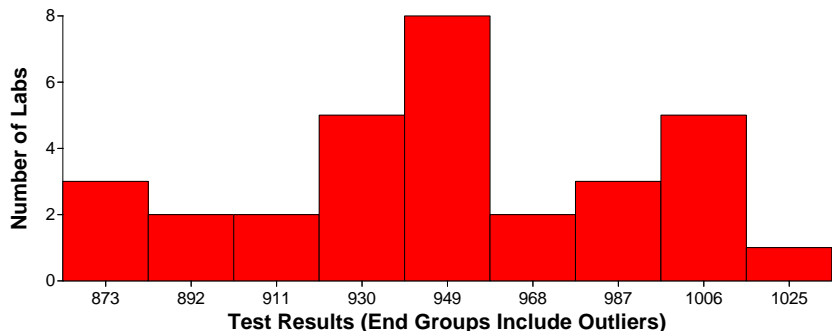


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 30 Fail: 1 Total: 31
 Totals for Matrix/Analyte: Labs: Pass: 63 Fail: 4 Total: 67

Potable Water Dalapon

Potable Water Dalapon

Shipment: 407 Matrix: Potable Water
Analyte: Dalapon
Sample: 0717
Technology: GC-ECD
Prep Method:
Target: 84.2 ug/L
Limits: 42.1 to 126 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 72.7 ug/L
Std Dev: 11.5613 ug/L
Median: 72.6 ug/L

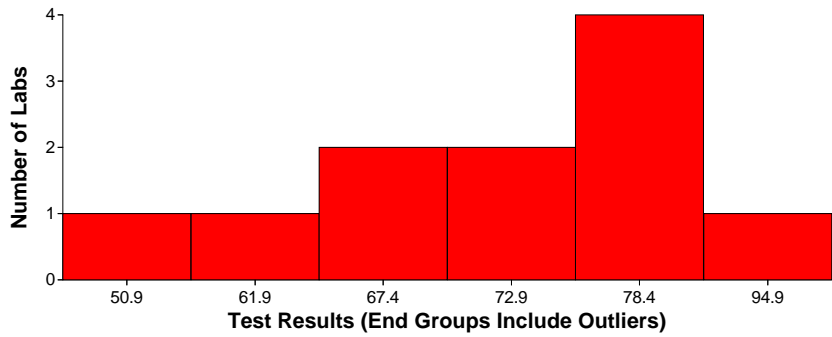


Totals for Matrix/Analyte/Technology:

Labs: Pass: 11 Fail: 0 Total: 11

Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water Dibromoacetic acid

Shipment: 407 Matrix: Potable Water
Analyte: Dibromoacetic acid
Sample: 0726
Technology: GC-ECD
Prep Method:
Target: 23.8 ug/L
Limits: 14.3 to 33.3 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 22.7 ug/L
Std Dev: 6.1824 ug/L
Median: 23.5 ug/L

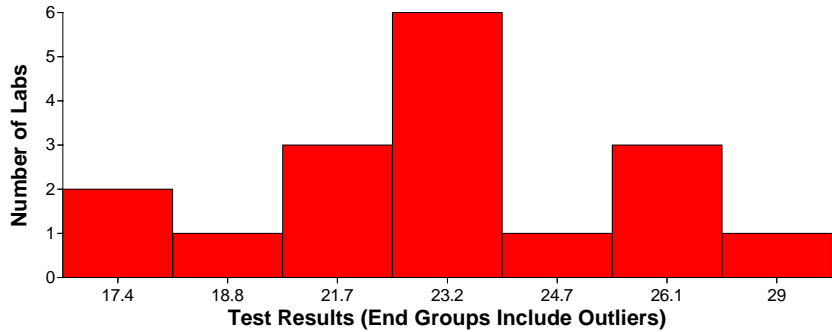

Totals for Matrix/Analyte/Technology:

Labs: Pass: 17 Fail: 0 Total: 17

Totals for Matrix/Analyte: Labs: Pass: 18 Fail: 0 Total: 18

Potable Water Dibromoacetic acid

Shipment: 407 Matrix: Potable Water
Analyte: Dibromoacetic acid
Sample: 0726
Technology: IC-ESI-MS
Prep Method:
Target: 23.8 ug/L
Limits: 14.3 to 33.3 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 24.3 ug/L
Std Dev: 0 ug/L
Median: 24.3 ug/L

A histogram is not displayed for Technology: IC-ESI-MS due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 18 Fail: 0 Total: 18

Potable Water Dichloroacetic acid

Shipment: 407 Matrix: Potable Water
Analyte: Dichloroacetic acid
Sample: 0726
Technology: GC-ECD
Prep Method:
Target: 16.2 ug/L
Limits: 9.72 to 22.7 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 15.5 ug/L
Std Dev: 1.8506 ug/L
Median: 15.6 ug/L

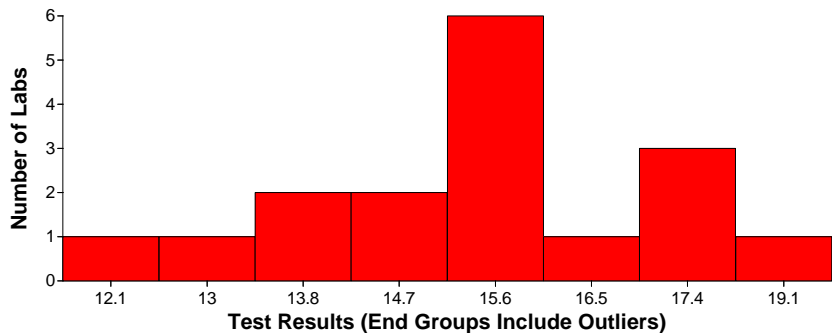

Totals for Matrix/Analyte/Technology:

Labs: Pass: 17 Fail: 0 Total: 17

Totals for Matrix/Analyte: Labs: Pass: 18 Fail: 0 Total: 18

Potable Water Dichloroacetic acid

Shipment: 407 Matrix: Potable Water
 Analyte: Dichloroacetic acid
 Sample: 0726
 Technology: IC-ESI-MS
 Prep Method:
 Target: 16.2 ug/L
 Limits: 9.72 to 22.7 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 16.5 ug/L
 Std Dev: 0 ug/L
 Median: 16.5 ug/L


A histogram is not displayed for Technology: IC-ESI-MS due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 18 Fail: 0 Total: 18

Potable Water Dichlorodifluoromethane

Shipment: 407 Matrix: Potable Water
 Analyte: Dichlorodifluoromethane
 Sample: 0720
 Technology: GC-MS
 Prep Method:
 Target: 11.2 ug/L
 Limits: 6.72 to 15.7 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 13.1 ug/L
 Std Dev: 2.45 ug/L
 Median: 12.3 ug/L

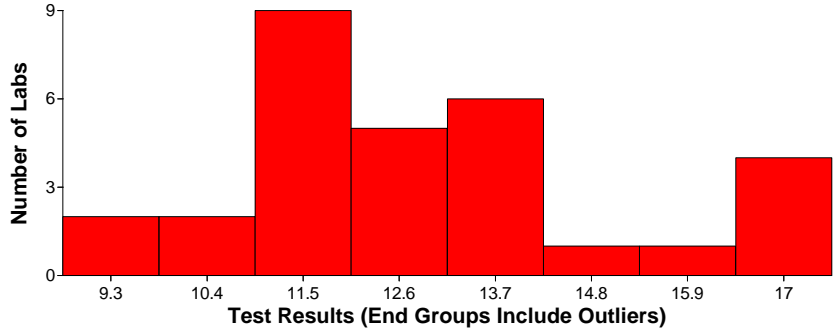

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 25 Fail: 5 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 26 Fail: 5 Total: 31

Potable Water Dichlorodifluoromethane

Shipment: 407 Matrix: Potable Water
 Analyte: Dichlorodifluoromethane
 Sample: 0720
 Technology: GCELCD/PID
 Prep Method:
 Target: 11.2 ug/L
 Limits: 6.72 to 15.7 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 10.4 ug/L
 Std Dev: 0 ug/L
 Median: 10.4 ug/L


A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 26 Fail: 5 Total: 31

Potable Water Dicamba

Shipment: 407 Matrix: Potable Water
 Analyte: Dicamba
 Sample: 0717
 Technology: GC-ECD
 Prep Method:
 Target: 57 ug/L
 Limits: 28.5 to 85.5 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 52.2 ug/L
 Std Dev: 8.4079 ug/L
 Median: 53.65 ug/L

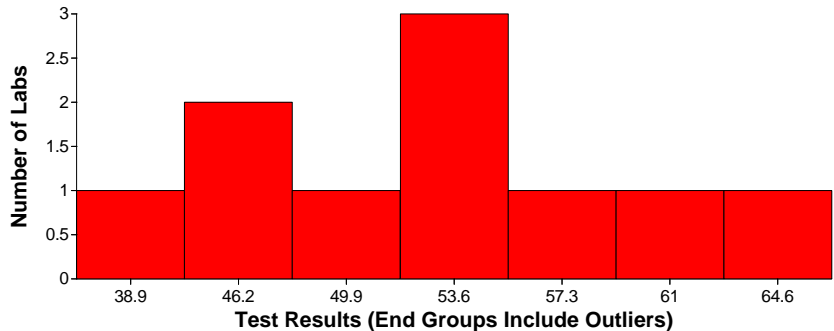

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 10 Fail: 0 Total: 10

Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water Dicamba

Shipment: 407 Matrix: Potable Water
Analyte: Dicamba
Sample: 0717
Technology: HPLC-UV
Prep Method:
Target: 57 ug/L
Limits: 28.5 to 85.5 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 58.1 ug/L
Std Dev: 0 ug/L
Median: 58.1 ug/L

A histogram is not displayed for
Technology: HPLC-UV due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water Dinoseb

Shipment: 407 Matrix: Potable Water
Analyte: Dinoseb
Sample: 0717
Technology: GC-ECD
Prep Method:
Target: 40.2 ug/L
Limits: 13.8 to 56.1 ug/L
Basis: Linear Regression
Robust Mean: 36.5 ug/L
Std Dev: 4.906 ug/L
Median: 37.85 ug/L

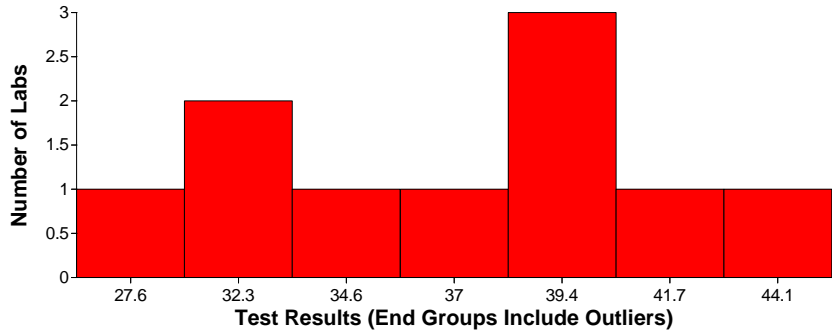

Totals for Matrix/Analyte/Technology:

Labs: Pass: 10 Fail: 0 Total: 10

Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water Dinoseb

Shipment: 407 Matrix: Potable Water
Analyte: Dinoseb
Sample: 0717
Technology: HPLC-UV
Prep Method:
Target: 40.2 ug/L
Limits: 13.8 to 56.1 ug/L
Basis: Linear Regression
Robust Mean: 39.5 ug/L
Std Dev: 0 ug/L
Median: 39.5 ug/L

A histogram is not displayed for
Technology: HPLC-UV due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water Diquat

Shipment: 407 Matrix: Potable Water
Analyte: Diquat
Sample: 0710
Technology: HPLC-UV
Prep Method:
Target: 24.6 ug/L
Limits: 12.3 to 36.9 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 20.7 ug/L
Std Dev: 3.7905 ug/L
Median: 19.8 ug/L

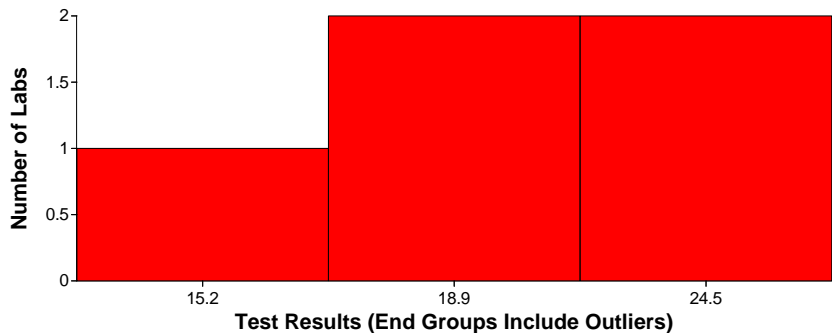

Totals for Matrix/Analyte/Technology:


Labs: Pass: 5 Fail: 0 Total: 5

Totals for Matrix/Analyte: Labs: Pass: 5 Fail: 0 Total: 5

Potable Water Organic Carbon, Dissolved

Potable Water Organic Carbon, Dissolved


Shipment: 407 **Matrix:** Potable Water
Analyte: Organic Carbon, Dissolved
Sample: 0733
Technology: IR
Prep Method:
Target: 2.79 mg/L
Limits: 2.45 to 3.18 mg/L
Basis: Linear Regression
Robust Mean: 2.9 mg/L
Std Dev: 0.3602 mg/L
Median: 2.855 mg/L

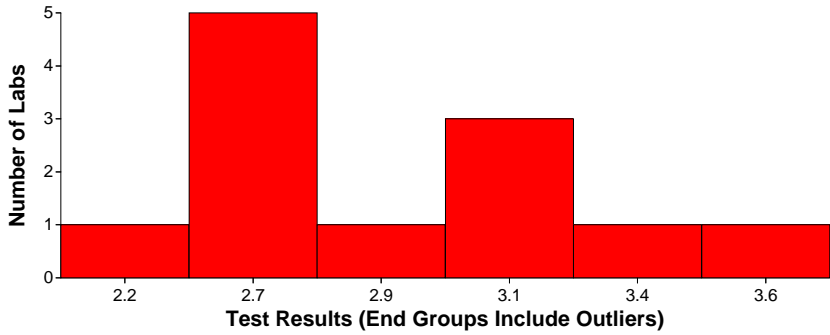

Totals for Matrix/Analyte/Technology:
Labs: Pass: 9 **Fail:** 3 **Total:** 12
Totals for Matrix/Analyte: **Labs: Pass:** 9 **Fail:** 3 **Total:** 12

Potable Water Endothall


Shipment: 407 **Matrix:** Potable Water
Analyte: Endothall
Sample: 0711
Technology: GC-MS
Prep Method:
Target: 163 ug/L
Limits: 81.5 to 245 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 159.3 ug/L
Std Dev: 28.5365 ug/L
Median: 170 ug/L

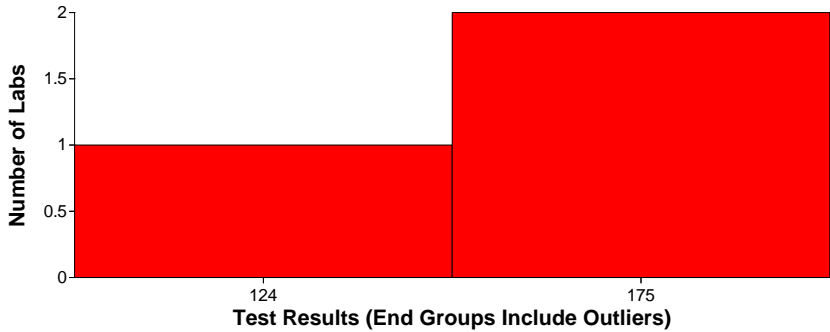

Totals for Matrix/Analyte/Technology:
Labs: Pass: 3 **Fail:** 0 **Total:** 3
Totals for Matrix/Analyte: **Labs: Pass:** 3 **Fail:** 0 **Total:** 3

Potable Water Endrin


Shipment: 407 **Matrix:** Potable Water
Analyte: Endrin
Sample: 0707A
Technology: GC-ECD
Prep Method:
Target: 1.46 ug/L
Limits: 1.02 to 1.9 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 1.4 ug/L
Std Dev: 0.1852 ug/L
Median: 1.43 ug/L

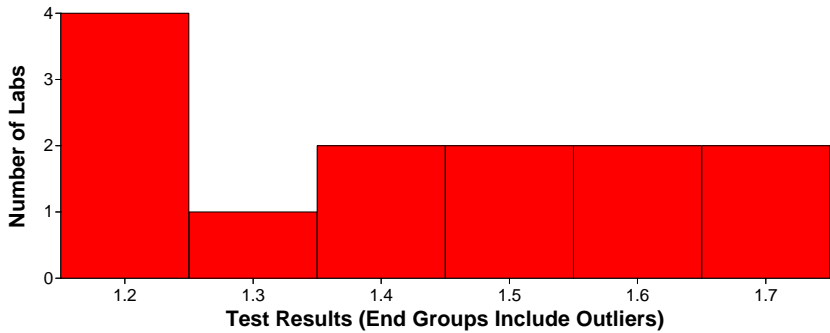

Totals for Matrix/Analyte/Technology:
Labs: Pass: 13 **Fail:** 0 **Total:** 13
Totals for Matrix/Analyte: **Labs: Pass:** 18 **Fail:** 0 **Total:** 18

Potable Water Endrin

Shipment: 407 **Matrix:** Potable Water
Analyte: Endrin
Sample: 0707A
Technology: GC-MS
Prep Method:
Target: 1.46 ug/L
Limits: 1.02 to 1.9 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 1.5 ug/L
Std Dev: 0.2329 ug/L
Median: 1.4 ug/L

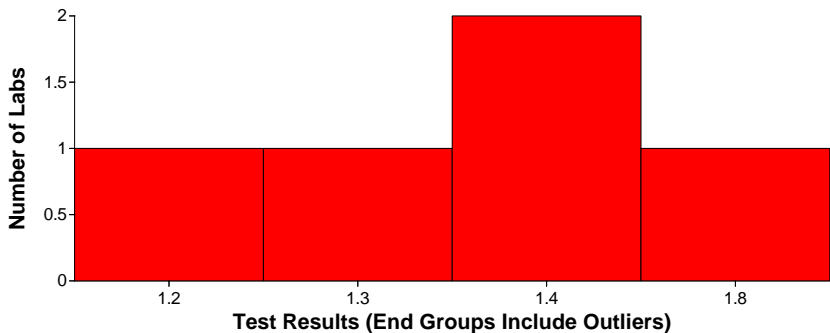


Totals for Matrix/Analyte/Technology:
Labs: Pass: 5 **Fail:** 0 **Total:** 5
Totals for Matrix/Analyte: **Labs: Pass:** 18 **Fail:** 0 **Total:** 18

Potable Water Ethyl benzene

Potable Water Ethyl benzene

Shipment: 407 Matrix: Potable Water
Analyte: Ethyl benzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 17.8 ug/L
Limits: 14.2 to 21.4 ug/L
Basis: Fixed Percent (2)
Robust Mean: 17.8 ug/L
Std Dev: 3.4922 ug/L
Median: 17.7 ug/L

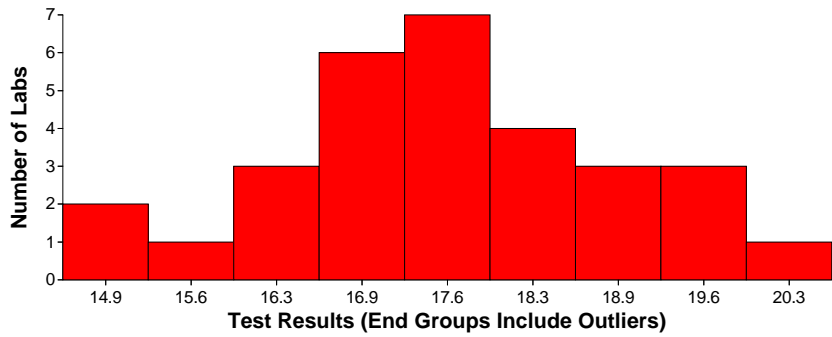

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water Ethyl benzene

Shipment: 407 Matrix: Potable Water
Analyte: Ethyl benzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 17.8 ug/L
Limits: 14.2 to 21.4 ug/L
Basis: Fixed Percent (2)
Robust Mean: 15.9 ug/L
Std Dev: 0 ug/L
Median: 15.9 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water Iron, Total

Shipment: 407 Matrix: Potable Water
Analyte: Iron, Total
Sample: 0706
Technology: FAAS
Prep Method:
Target: 1100 ug/L
Limits: 935 to 1270 ug/L
Basis: Fixed Percent (2)
Robust Mean: 1115.5 ug/L
Std Dev: 518.3126 ug/L
Median: 1104.5 ug/L

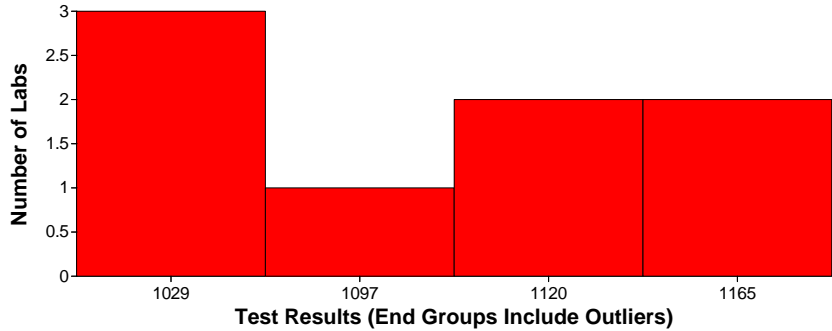

Totals for Matrix/Analyte/Technology:

Labs: Pass: 6 Fail: 2 Total: 8

Totals for Matrix/Analyte: Labs: Pass: 41 Fail: 3 Total: 44

Potable Water Iron, Total

Shipment: 407 Matrix: Potable Water
Analyte: Iron, Total
Sample: 0706
Technology: GFAAS
Prep Method:
Target: 1100 ug/L
Limits: 935 to 1270 ug/L
Basis: Fixed Percent (2)
Robust Mean: 1140 ug/L
Std Dev: 0 ug/L
Median: 1140 ug/L

A histogram is not displayed for Technology: GFAAS due to the limited number of participants.

Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1


Totals for Matrix/Analyte: Labs: Pass: 41 Fail: 3 Total: 44

Potable Water Iron, Total

Potable Water Iron, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Iron, Total
 Sample: 0706
 Technology: ICP-AES
 Prep Method:
 Target: 1100 ug/L
 Limits: 935 to 1270 ug/L
 Basis: Fixed Percent (2)
 Robust Mean: 1116.2 ug/L
 Std Dev: 323.9325 ug/L
 Median: 1120 ug/L

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 33 Fail: 1 Total: 34
 Totals for Matrix/Analyte: Labs: Pass: 41 Fail: 3 Total: 44

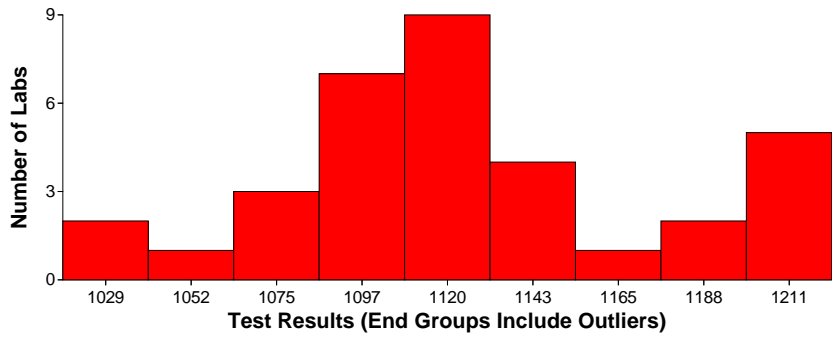

Potable Water Iron, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Iron, Total
 Sample: 0706
 Technology: ICP-MS
 Prep Method:
 Target: 1100 ug/L
 Limits: 935 to 1270 ug/L
 Basis: Fixed Percent (2)
 Robust Mean: 1129 ug/L
 Std Dev: 0 ug/L
 Median: 1129 ug/L

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 1 Fail: 0 Total: 1
 Totals for Matrix/Analyte: Labs: Pass: 41 Fail: 3 Total: 44

A histogram is not displayed for Technology: ICP-MS due to the limited number of participants.

Potable Water Fluoride, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Fluoride, Total
 Sample: 0702
 Technology: COLOR
 Prep Method:
 Target: 3.15 mg/L
 Limits: 2.84 to 3.47 mg/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 3.3 mg/L
 Std Dev: 0.1838 mg/L
 Median: 3.33 mg/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 2 Fail: 0 Total: 2
 Totals for Matrix/Analyte: Labs: Pass: 55 Fail: 3 Total: 58

A histogram is not displayed for Technology: COLOR due to the limited number of participants.

Potable Water Fluoride, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Fluoride, Total
 Sample: 0702
 Technology: IC-COND
 Prep Method:
 Target: 3.15 mg/L
 Limits: 2.84 to 3.47 mg/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 3.1 mg/L
 Std Dev: 0.7967 mg/L
 Median: 3.13 mg/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 29 Fail: 2 Total: 31
 Totals for Matrix/Analyte: Labs: Pass: 55 Fail: 3 Total: 58

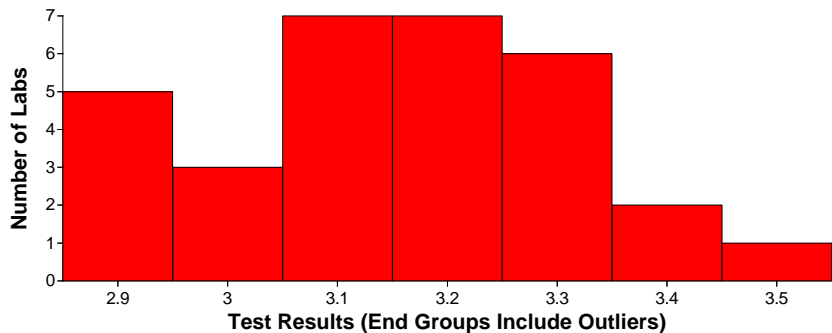

Potable Water Fluoride, Total

Potable Water Fluoride, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Fluoride, Total
Sample: 0702
Technology: POT
Prep Method:
Target: 3.15 mg/L
Limits: 2.84 to 3.47 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 3.2 mg/L
Std Dev: 0.1429 mg/L
Median: 3.16 mg/L

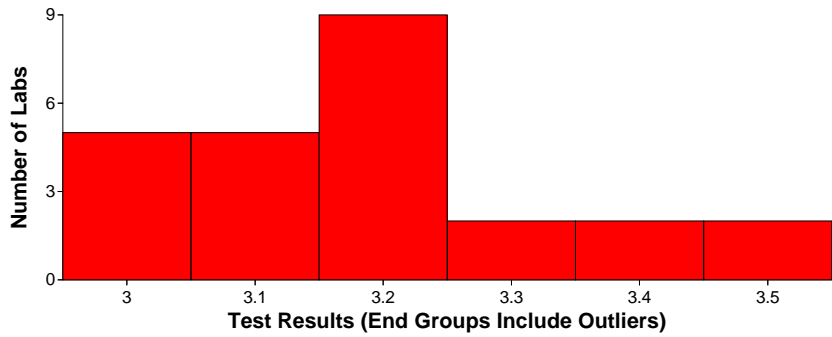


Totals for Matrix/Analyte/Technology:

Labs: Pass: 24 Fail: 1 Total: 25

Totals for Matrix/Analyte: Labs: Pass: 55 Fail: 3 Total: 58

Potable Water Glyphosate

Shipment: 407 **Matrix:** Potable Water
Analyte: Glyphosate
Sample: 0712
Technology: HPLC-UV
Prep Method:
Target: 653 ug/L
Limits: 522 to 784 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 639 ug/L
Std Dev: 43.3036 ug/L
Median: 648.55 ug/L

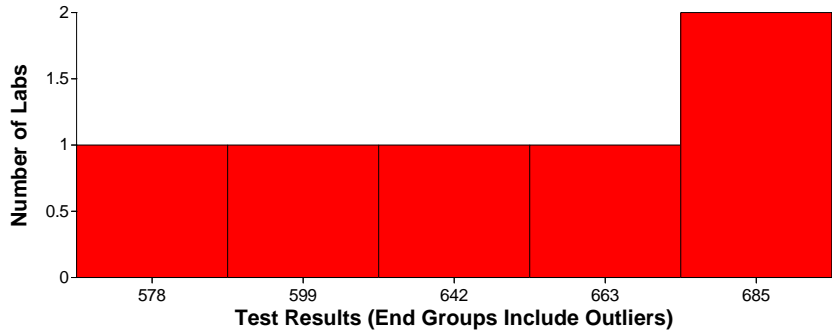


Totals for Matrix/Analyte/Technology:

Labs: Pass: 6 Fail: 0 Total: 6

Totals for Matrix/Analyte: Labs: Pass: 6 Fail: 0 Total: 6

Potable Water Hexachlorobenzene

Shipment: 407 **Matrix:** Potable Water
Analyte: Hexachlorobenzene
Sample: 0707A
Technology: GC-ECD
Prep Method:
Target: 1.22 ug/L
Limits: 0.593 to 1.55 ug/L
Basis: Linear Regression
Robust Mean: 1.2 ug/L
Std Dev: 0.129 ug/L
Median: 1.12 ug/L

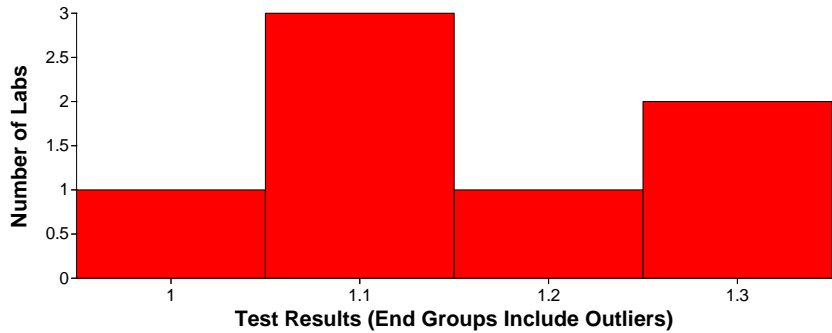


Totals for Matrix/Analyte/Technology:

Labs: Pass: 7 Fail: 0 Total: 7

Totals for Matrix/Analyte: Labs: Pass: 16 Fail: 0 Total: 16

Potable Water Hexachlorobenzene

Shipment: 407 **Matrix:** Potable Water
Analyte: Hexachlorobenzene
Sample: 0707A
Technology: GC-MS
Prep Method:
Target: 1.22 ug/L
Limits: 0.593 to 1.55 ug/L
Basis: Linear Regression
Robust Mean: 1.2 ug/L
Std Dev: 0.4071 ug/L
Median: 1.2 ug/L

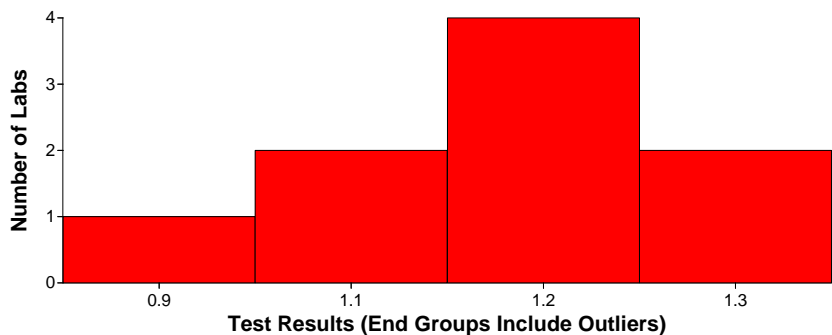

Totals for Matrix/Analyte/Technology:


Labs: Pass: 9 Fail: 0 Total: 9

Totals for Matrix/Analyte: Labs: Pass: 16 Fail: 0 Total: 16

Potable Water Hexachlorobutadiene

Potable Water Hexachlorobutadiene

Shipment: 407 **Matrix:** Potable Water
Analyte: Hexachlorobutadiene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 31.3 ug/L
Limits: 25 to 37.6 ug/L
Basis: Fixed Percent (2)
Robust Mean: 31.3 ug/L
Std Dev: 6.5171 ug/L
Median: 30.75 ug/L

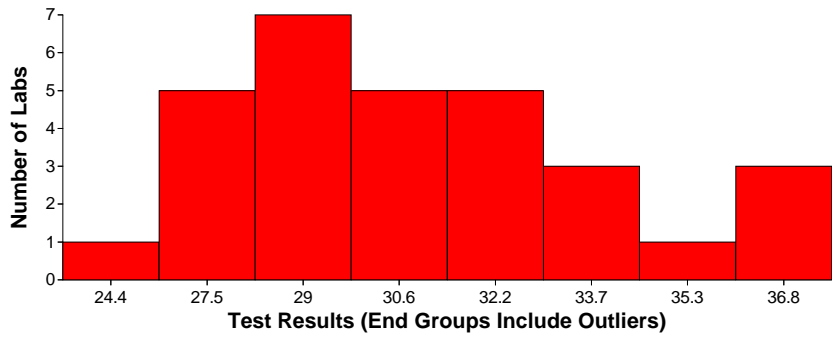

Totals for Matrix/Analyte/Technology:

Labs: Pass: 27 **Fail:** 3 **Total:** 30

Totals for Matrix/Analyte: **Labs: Pass:** 28 **Fail:** 3 **Total:** 31

Potable Water Hexachlorobutadiene

Shipment: 407 **Matrix:** Potable Water
Analyte: Hexachlorobutadiene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 31.3 ug/L
Limits: 25 to 37.6 ug/L
Basis: Fixed Percent (2)
Robust Mean: 26.5 ug/L
Std Dev: 0 ug/L
Median: 26.5 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 **Fail:** 0 **Total:** 1

Totals for Matrix/Analyte: **Labs: Pass:** 28 **Fail:** 3 **Total:** 31

Potable Water Hexachlorocyclopentadiene

Shipment: 407 **Matrix:** Potable Water
Analyte: Hexachlorocyclopentadiene
Sample: 0707A
Technology: GC-ECD
Prep Method:
Target: 11.8 ug/L
Limits: 3.5 to 16.8 ug/L
Basis: Linear Regression
Robust Mean: 11.4 ug/L
Std Dev: 1.4425 ug/L
Median: 11.75 ug/L

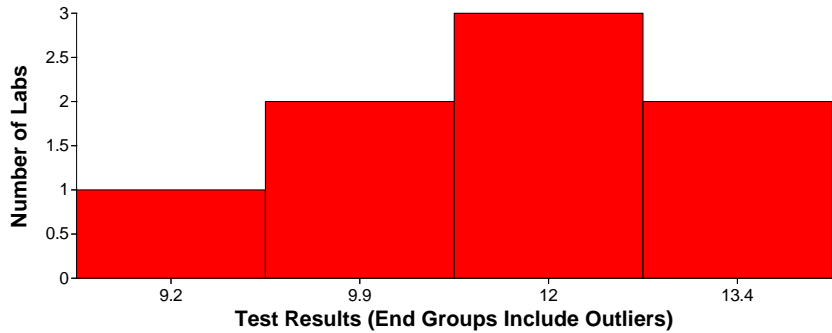


Totals for Matrix/Analyte/Technology:

Labs: Pass: 8 **Fail:** 0 **Total:** 8

Totals for Matrix/Analyte: **Labs: Pass:** 16 **Fail:** 1 **Total:** 17

Potable Water Hexachlorocyclopentadiene

Shipment: 407 **Matrix:** Potable Water
Analyte: Hexachlorocyclopentadiene
Sample: 0707A
Technology: GC-MS
Prep Method:
Target: 11.8 ug/L
Limits: 3.5 to 16.8 ug/L
Basis: Linear Regression
Robust Mean: 11.6 ug/L
Std Dev: 4.157 ug/L
Median: 10.8 ug/L

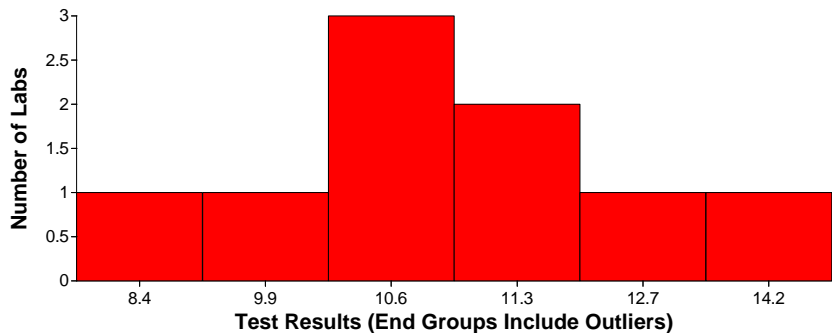

Totals for Matrix/Analyte/Technology:


Labs: Pass: 8 **Fail:** 1 **Total:** 9

Totals for Matrix/Analyte: **Labs: Pass:** 16 **Fail:** 1 **Total:** 17

Potable Water Heptachlor

Potable Water Heptachlor

Shipment: 407 **Matrix:** Potable Water
Analyte: Heptachlor
Sample: 0707A
Technology: GC-ECD
Prep Method:
Target: 0.702 ug/L
Limits: 0.386 to 1.02 ug/L
Basis: Target Value +/- a percent
Robust Mean: 0.7 ug/L
Std Dev: 0.0756 ug/L
Median: 0.665 ug/L

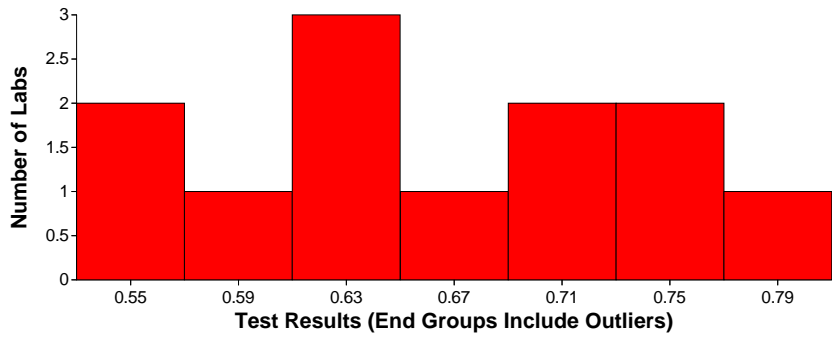


Totals for Matrix/Analyte/Technology:

Labs: Pass: 12 **Fail:** 0 **Total:** 12

Totals for Matrix/Analyte: **Labs: Pass:** 16 **Fail:** 0 **Total:** 16

Potable Water Heptachlor

Shipment: 407 **Matrix:** Potable Water
Analyte: Heptachlor
Sample: 0707A
Technology: GC-MS
Prep Method:
Target: 0.702 ug/L
Limits: 0.386 to 1.02 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 0.7 ug/L
Std Dev: 0.0838 ug/L
Median: 0.695 ug/L

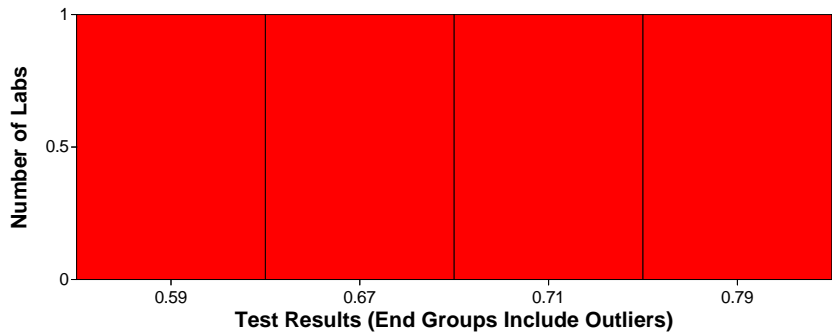


Totals for Matrix/Analyte/Technology:

Labs: Pass: 4 **Fail:** 0 **Total:** 4

Totals for Matrix/Analyte: **Labs: Pass:** 16 **Fail:** 0 **Total:** 16

Potable Water Heptachlor epoxide

Shipment: 407 **Matrix:** Potable Water
Analyte: Heptachlor epoxide
Sample: 0707A
Technology: GC-ECD
Prep Method:
Target: 2.16 ug/L
Limits: 1.19 to 3.13 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 2.1 ug/L
Std Dev: 0.2602 ug/L
Median: 2.105 ug/L

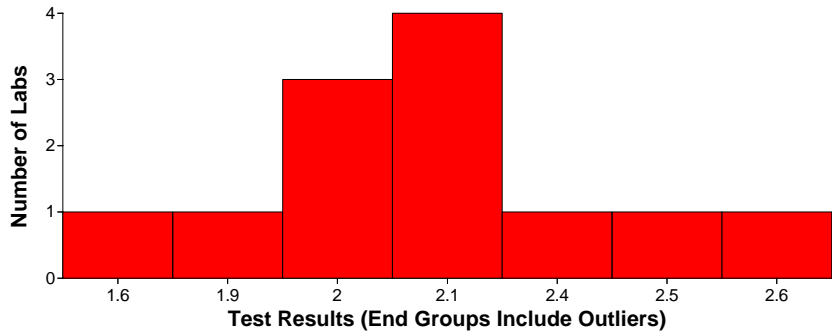


Totals for Matrix/Analyte/Technology:

Labs: Pass: 12 **Fail:** 0 **Total:** 12

Totals for Matrix/Analyte: **Labs: Pass:** 18 **Fail:** 0 **Total:** 18

Potable Water Heptachlor epoxide

Shipment: 407 **Matrix:** Potable Water
Analyte: Heptachlor epoxide
Sample: 0707A
Technology: GC-MS
Prep Method:
Target: 2.16 ug/L
Limits: 1.19 to 3.13 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 2.1 ug/L
Std Dev: 0.2975 ug/L
Median: 2.13 ug/L

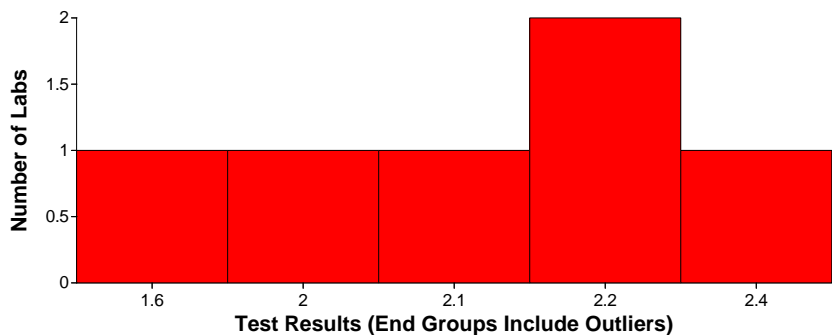

Totals for Matrix/Analyte/Technology:

Labs: Pass: 6 **Fail:** 0 **Total:** 6

Totals for Matrix/Analyte: **Labs: Pass:** 18 **Fail:** 0 **Total:** 18

Potable Water Mercury, Total


Potable Water Mercury, Total

Shipment: 407 Matrix: Potable Water
Analyte: Mercury, Total
Sample: 0706
Technology: CVAAS
Prep Method:
Target: 7.52 ug/L
Limits: 5.26 to 9.78 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 6.9 ug/L
Std Dev: 0.6446 ug/L
Median: 6.775 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 26 Fail: 0 Total: 26

Totals for Matrix/Analyte: Labs: Pass: 37 Fail: 0 Total: 37

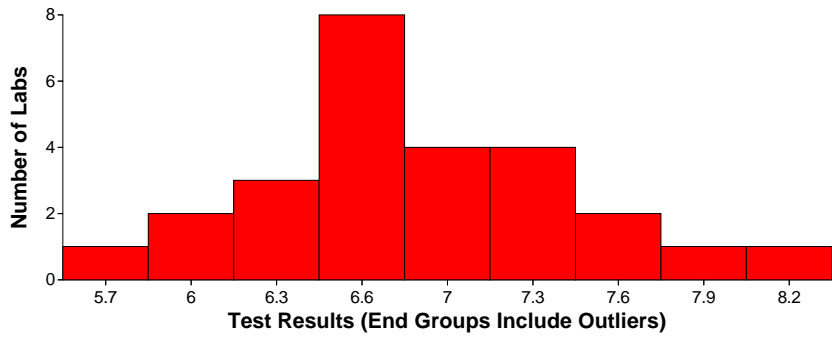


Potable Water Mercury, Total

Shipment: 407 Matrix: Potable Water
Analyte: Mercury, Total
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 7.52 ug/L
Limits: 5.26 to 9.78 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 7.2 ug/L
Std Dev: 0.8046 ug/L
Median: 7.32 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 11 Fail: 0 Total: 11

Totals for Matrix/Analyte: Labs: Pass: 37 Fail: 0 Total: 37

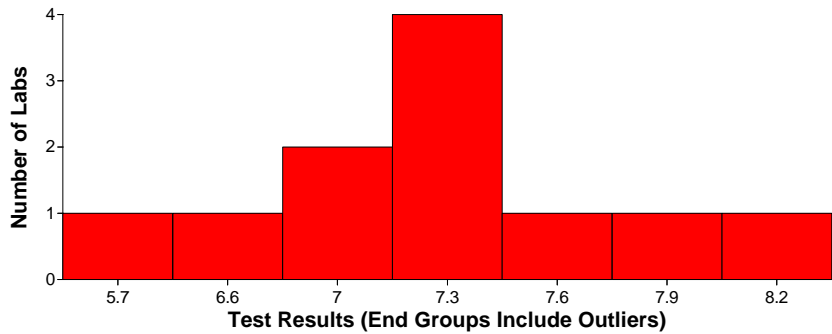


Potable Water Isopropylbenzene

Shipment: 407 Matrix: Potable Water
Analyte: Isopropylbenzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 19.3 ug/L
Limits: 15.4 to 23.2 ug/L
Basis: Fixed Percent (2)
Robust Mean: 19.7 ug/L
Std Dev: 3.9419 ug/L
Median: 19.55 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

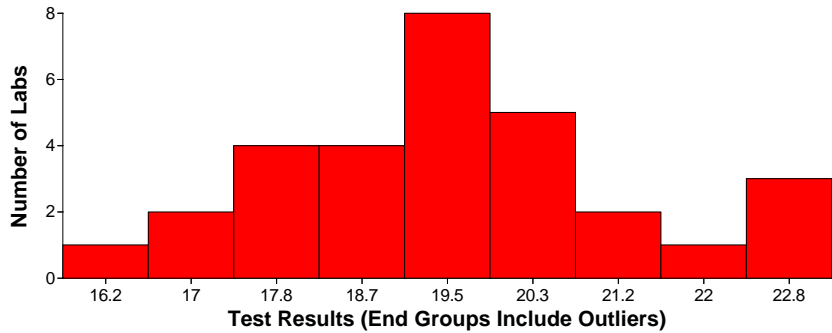

Potable Water Isopropylbenzene

Shipment: 407 Matrix: Potable Water
Analyte: Isopropylbenzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 19.3 ug/L
Limits: 15.4 to 23.2 ug/L
Basis: Fixed Percent (2)
Robust Mean: 16.7 ug/L
Std Dev: 0 ug/L
Median: 16.7 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Potable Water Potassium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Potassium, Total
Sample: 0732
Technology: IC
Prep Method:
Target: 20.2 mg/L
Limits: 17.2 to 23.2 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 18 mg/L
Std Dev: 0 mg/L
Median: 18 mg/L

A histogram is not displayed for
Technology: IC due to the limited
number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 27 Fail: 1 Total: 28

Potable Water Potassium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Potassium, Total
Sample: 0732
Technology: ICP-AES
Prep Method:
Target: 20.2 mg/L
Limits: 17.2 to 23.2 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 20.3 mg/L
Std Dev: 4.1166 mg/L
Median: 20.45 mg/L

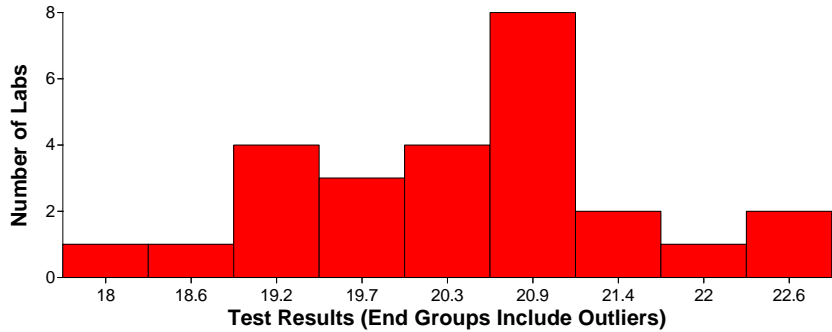

Totals for Matrix/Analyte/Technology:

Labs: Pass: 25 Fail: 1 Total: 26

Totals for Matrix/Analyte: Labs: Pass: 27 Fail: 1 Total: 28

Potable Water Potassium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Potassium, Total
Sample: 0732
Technology: ICP-MS
Prep Method:
Target: 20.2 mg/L
Limits: 17.2 to 23.2 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 21.2 mg/L
Std Dev: 0 mg/L
Median: 21.2 mg/L

A histogram is not displayed for
Technology: ICP-MS due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 27 Fail: 1 Total: 28

Potable Water Lindane

Shipment: 407 Matrix: Potable Water
Analyte: Lindane
Sample: 0707A
Technology: GC-ECD
Prep Method:
Target: 1.29 ug/L
Limits: 0.71 to 1.87 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 1.3 ug/L
Std Dev: 0.1413 ug/L
Median: 1.215 ug/L

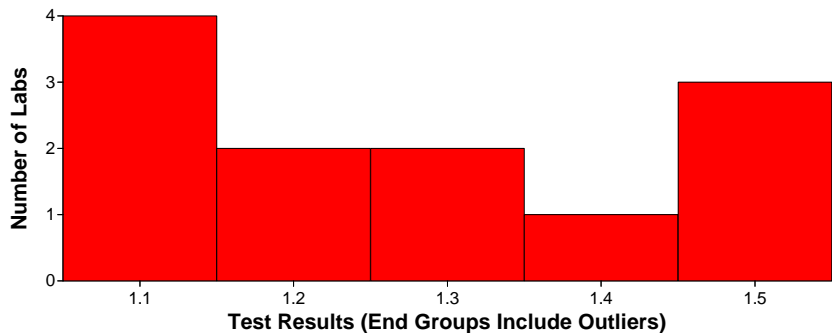

Totals for Matrix/Analyte/Technology:


Labs: Pass: 12 Fail: 0 Total: 12

Totals for Matrix/Analyte: Labs: Pass: 18 Fail: 0 Total: 18

Potable Water Lindane

Potable Water Lindane

Shipment: 407 Matrix: Potable Water
Analyte: Lindane
Sample: 0707A
Technology: GC-MS
Prep Method:
Target: 1.29 ug/L
Limits: 0.71 to 1.87 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 1.3 ug/L
Std Dev: 0.525 ug/L
Median: 1.28 ug/L

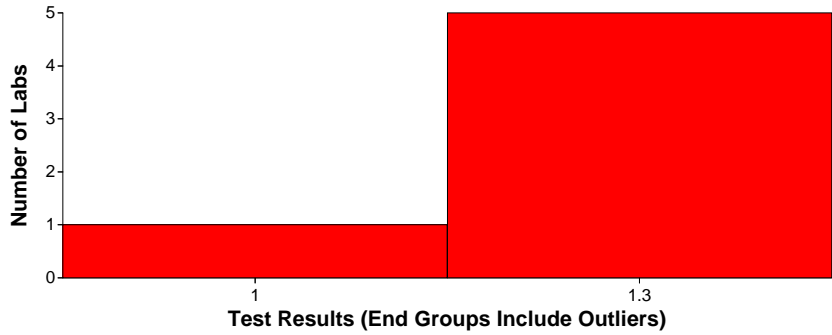


Totals for Matrix/Analyte/Technology:

Labs: Pass: 6 Fail: 0 Total: 6

Totals for Matrix/Analyte: Labs: Pass: 18 Fail: 0 Total: 18

Potable Water Monobromoacetic acid

Shipment: 407 Matrix: Potable Water
Analyte: Monobromoacetic acid
Sample: 0726
Technology: GC-ECD
Prep Method:
Target: 22.2 ug/L
Limits: 13.3 to 31.1 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 20.6 ug/L
Std Dev: 5.2773 ug/L
Median: 21 ug/L

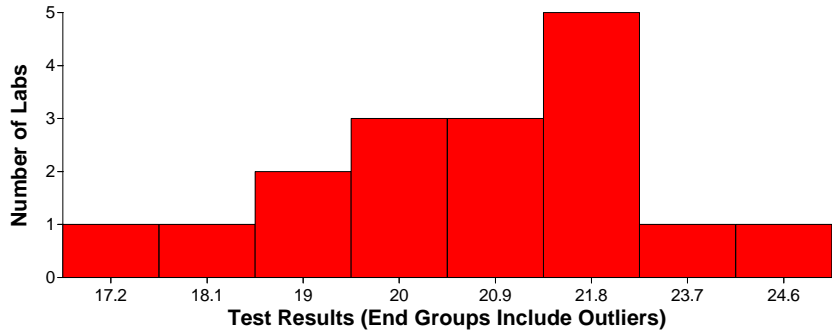

Totals for Matrix/Analyte/Technology:

Labs: Pass: 17 Fail: 0 Total: 17

Totals for Matrix/Analyte: Labs: Pass: 18 Fail: 0 Total: 18

Potable Water Monobromoacetic acid

Shipment: 407 Matrix: Potable Water
Analyte: Monobromoacetic acid
Sample: 0726
Technology: IC-ESI-MS
Prep Method:
Target: 22.2 ug/L
Limits: 13.3 to 31.1 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 21.8 ug/L
Std Dev: 0 ug/L
Median: 21.8 ug/L

A histogram is not displayed for Technology: IC-ESI-MS due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 18 Fail: 0 Total: 18

Potable Water Monochloroacetic acid

Shipment: 407 Matrix: Potable Water
Analyte: Monochloroacetic acid
Sample: 0726
Technology: GC-ECD
Prep Method:
Target: 20.5 ug/L
Limits: 12.3 to 28.7 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 19.9 ug/L
Std Dev: 1.733 ug/L
Median: 19.9 ug/L

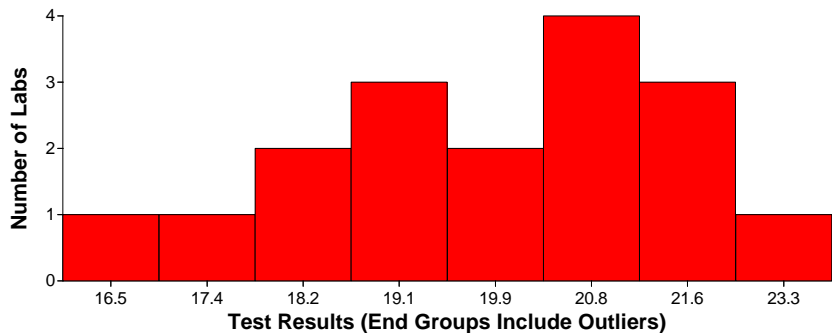

Totals for Matrix/Analyte/Technology:

Labs: Pass: 17 Fail: 0 Total: 17

Totals for Matrix/Analyte: Labs: Pass: 18 Fail: 0 Total: 18

Potable Water Monochloroacetic acid

Shipment: 407 Matrix: Potable Water
Analyte: Monochloroacetic acid
Sample: 0726
Technology: IC-ESI-MS
Prep Method:
Target: 20.5 ug/L
Limits: 12.3 to 28.7 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 19 ug/L
Std Dev: 0 ug/L
Median: 19 ug/L

A histogram is not displayed for
Technology: IC-ESI-MS due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 18 Fail: 0 Total: 18

Potable Water Methylene chloride

Shipment: 407 Matrix: Potable Water
Analyte: Methylene chloride
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 7.1 ug/L
Limits: 4.26 to 9.94 ug/L
Basis: Fixed Percent (2)
Robust Mean: 7.5 ug/L
Std Dev: 1.4371 ug/L
Median: 7.45 ug/L

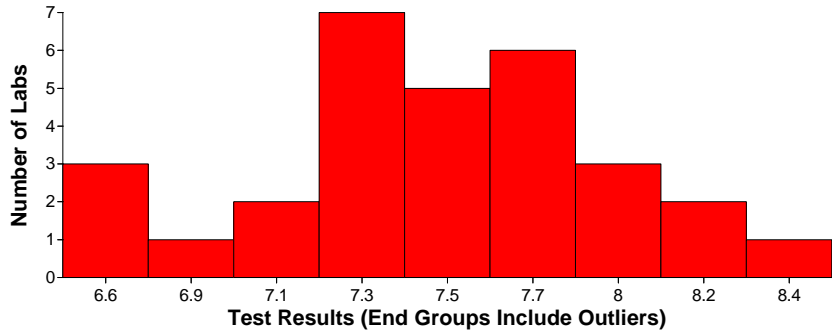

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water Methylene chloride

Shipment: 407 Matrix: Potable Water
Analyte: Methylene chloride
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 7.1 ug/L
Limits: 4.26 to 9.94 ug/L
Basis: Fixed Percent (2)
Robust Mean: 7.7 ug/L
Std Dev: 0 ug/L
Median: 7.68 ug/L

A histogram is not displayed for
Technology: GCELCD/PID due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water Methomyl

Shipment: 407 Matrix: Potable Water
Analyte: Methomyl
Sample: 0715
Technology: HPLC-FLUOR
Prep Method:
Target: 95.3 ug/L
Limits: 76.2 to 114 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 96 ug/L
Std Dev: 4.8099 ug/L
Median: 93.7 ug/L

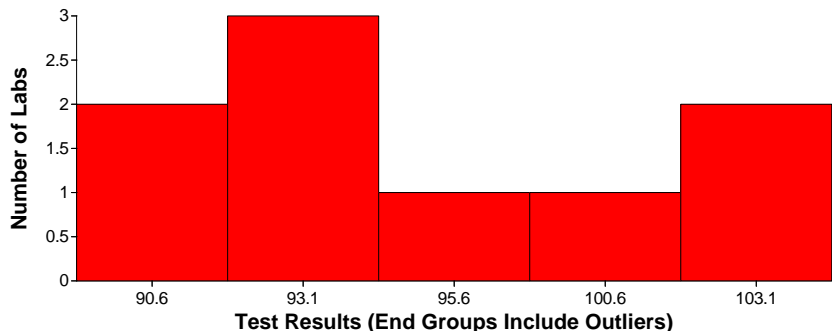

Totals for Matrix/Analyte/Technology:


Labs: Pass: 9 Fail: 0 Total: 9

Totals for Matrix/Analyte: Labs: Pass: 9 Fail: 0 Total: 9

Potable Water Metolachlor

Potable Water Metolachlor

Shipment: 407 **Matrix:** Potable Water
Analyte: Metolachlor
Sample: 0707B
Technology: GC-MS
Prep Method:
Target: 17.5 ug/L
Limits: 9.63 to 25.4 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 17.5 ug/L
Std Dev: 2.8931 ug/L
Median: 16.3 ug/L

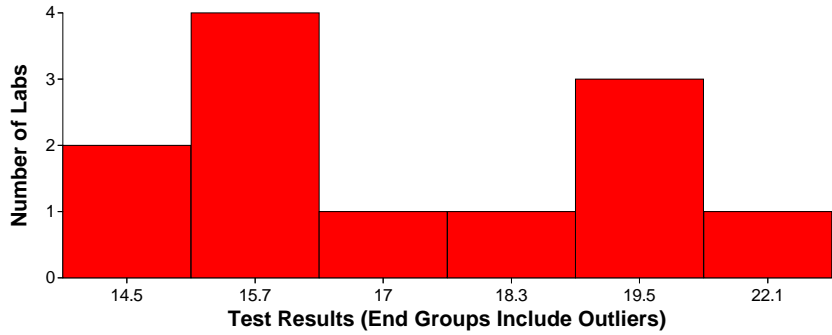

Totals for Matrix/Analyte/Technology:

Labs: Pass: 12 **Fail:** 0 **Total:** 12

Totals for Matrix/Analyte: **Labs: Pass:** 12 **Fail:** 0 **Total:** 12

Potable Water Metribuzin

Shipment: 407 **Matrix:** Potable Water
Analyte: Metribuzin
Sample: 0707B
Technology: GC-ECD
Prep Method:
Target: 6.12 ug/L
Limits: 3.06 to 9.18 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 6.8 ug/L
Std Dev: 0 ug/L
Median: 6.82 ug/L

A histogram is not displayed for Technology: GC-ECD due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 **Fail:** 0 **Total:** 1

Totals for Matrix/Analyte: **Labs: Pass:** 12 **Fail:** 0 **Total:** 12

Potable Water Metribuzin

Shipment: 407 **Matrix:** Potable Water
Analyte: Metribuzin
Sample: 0707B
Technology: GC-MS
Prep Method:
Target: 6.12 ug/L
Limits: 3.06 to 9.18 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 5.5 ug/L
Std Dev: 0.6245 ug/L
Median: 5.47 ug/L

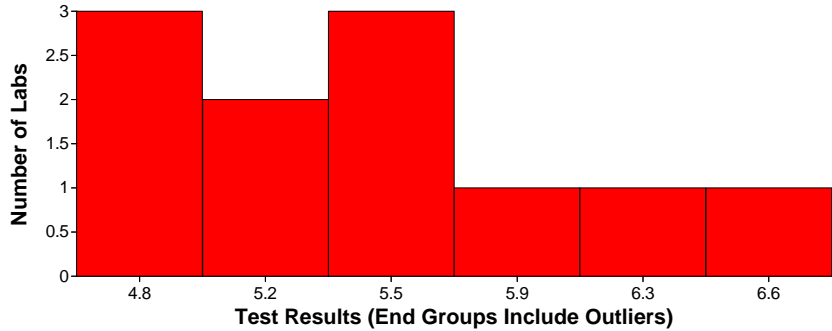


Totals for Matrix/Analyte/Technology:

Labs: Pass: 11 **Fail:** 0 **Total:** 11

Totals for Matrix/Analyte: **Labs: Pass:** 12 **Fail:** 0 **Total:** 12

Potable Water Magnesium, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Magnesium, Total
Sample: 0732
Technology: FAAS
Prep Method:
Target: 11.5 mg/L
Limits: 9.78 to 13.2 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 11.3 mg/L
Std Dev: 0.4133 mg/L
Median: 11.4 mg/L

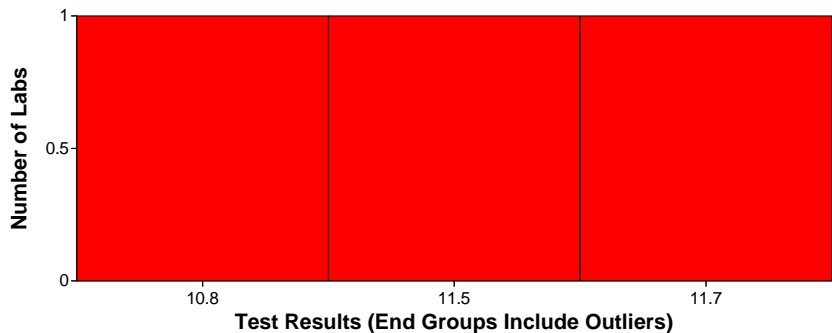

Totals for Matrix/Analyte/Technology:

Labs: Pass: 3 **Fail:** 0 **Total:** 3

Totals for Matrix/Analyte: **Labs: Pass:** 36 **Fail:** 0 **Total:** 36

Potable Water Magnesium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Magnesium, Total
Sample: 0732
Technology: IC
Prep Method:
Target: 11.5 mg/L
Limits: 9.78 to 13.2 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 10.5 mg/L
Std Dev: 0 mg/L
Median: 10.5 mg/L

A histogram is not displayed for Technology: IC due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 36 Fail: 0 Total: 36

Potable Water Magnesium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Magnesium, Total
Sample: 0732
Technology: ICP-AES
Prep Method:
Target: 11.5 mg/L
Limits: 9.78 to 13.2 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 11.5 mg/L
Std Dev: 0.461 mg/L
Median: 11.5 mg/L

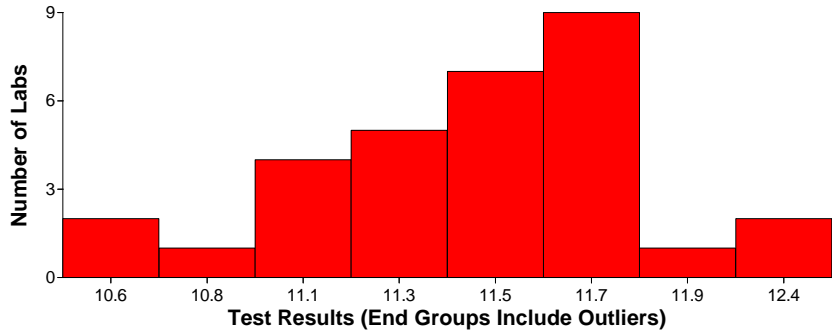

Totals for Matrix/Analyte/Technology:

Labs: Pass: 31 Fail: 0 Total: 31

Totals for Matrix/Analyte: Labs: Pass: 36 Fail: 0 Total: 36

Potable Water Magnesium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Magnesium, Total
Sample: 0732
Technology: ICP-MS
Prep Method:
Target: 11.5 mg/L
Limits: 9.78 to 13.2 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 11.9 mg/L
Std Dev: 0 mg/L
Median: 11.9 mg/L

A histogram is not displayed for Technology: ICP-MS due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 36 Fail: 0 Total: 36

Potable Water Manganese, Total

Shipment: 407 Matrix: Potable Water
Analyte: Manganese, Total
Sample: 0706
Technology: FAAS
Prep Method:
Target: 524 ug/L
Limits: 445 to 603 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 510 ug/L
Std Dev: 25.1794 ug/L
Median: 504 ug/L

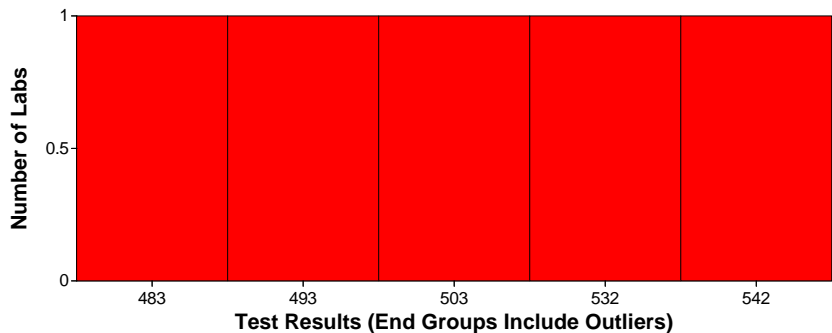

Totals for Matrix/Analyte/Technology:

Labs: Pass: 5 Fail: 0 Total: 5


Totals for Matrix/Analyte: Labs: Pass: 53 Fail: 2 Total: 55

Potable Water Manganese, Total

Potable Water Manganese, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Manganese, Total
Sample: 0706
Technology: ICP-AES
Prep Method:
Target: 524 ug/L
Limits: 445 to 603 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 528.5 ug/L
Std Dev: 103.2577 ug/L
Median: 530 ug/L


Totals for Matrix/Analyte/Technology:
Labs: Pass: 26 **Fail:** 1 **Total:** 27
Totals for Matrix/Analyte: **Labs: Pass:** 53 **Fail:** 2 **Total:** 55

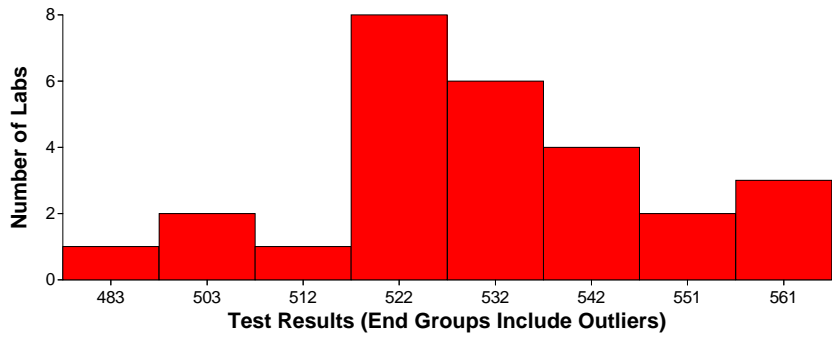

Potable Water Manganese, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Manganese, Total
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 524 ug/L
Limits: 445 to 603 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 516 ug/L
Std Dev: 108.8605 ug/L
Median: 511 ug/L


Totals for Matrix/Analyte/Technology:
Labs: Pass: 22 **Fail:** 1 **Total:** 23
Totals for Matrix/Analyte: **Labs: Pass:** 53 **Fail:** 2 **Total:** 55

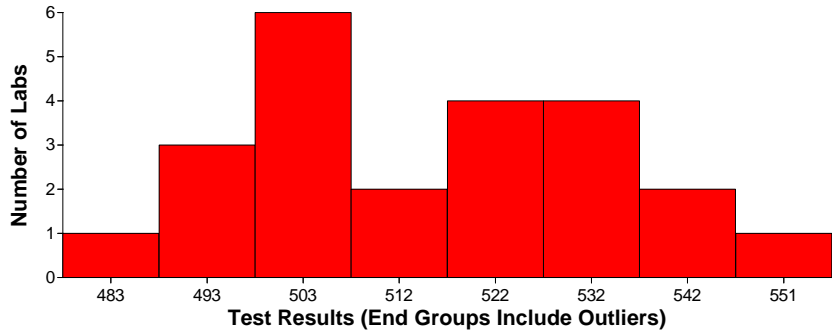

Potable Water Molybdenum, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Molybdenum, Total
Sample: 0706
Technology: ICP-AES
Prep Method:
Target: 80.1 ug/L
Limits: 68.1 to 92.1 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 76.1 ug/L
Std Dev: 2.1035 ug/L
Median: 76.1 ug/L


Totals for Matrix/Analyte/Technology:
Labs: Pass: 11 **Fail:** 0 **Total:** 11
Totals for Matrix/Analyte: **Labs: Pass:** 26 **Fail:** 0 **Total:** 26

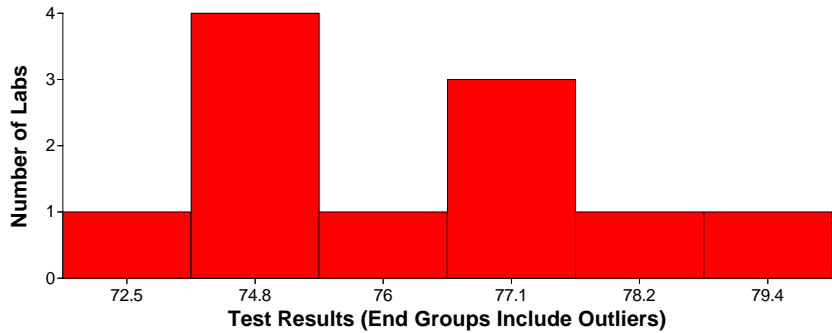

Potable Water Molybdenum, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Molybdenum, Total
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 80.1 ug/L
Limits: 68.1 to 92.1 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 77.8 ug/L
Std Dev: 2.2109 ug/L
Median: 78.2 ug/L


Totals for Matrix/Analyte/Technology:
Labs: Pass: 15 **Fail:** 0 **Total:** 15
Totals for Matrix/Analyte: **Labs: Pass:** 26 **Fail:** 0 **Total:** 26

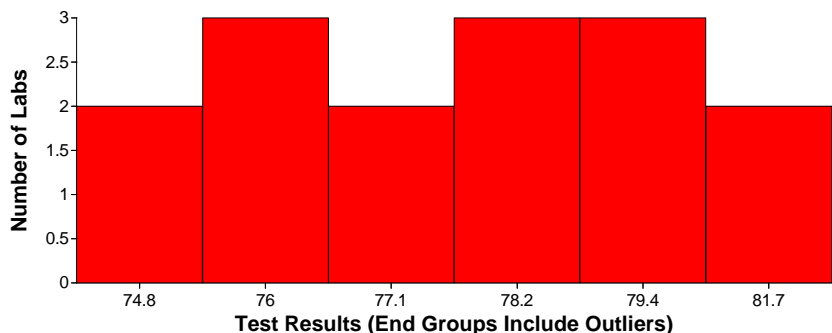

Potable Water Methyl tert-butyl ether

Potable Water Methyl tert-butyl ether

Shipment: 407 Matrix: Potable Water
Analyte: Methyl tert-butyl ether
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 47.2 ug/L
Limits: 37.8 to 56.6 ug/L
Basis: Fixed Percent (2)
Robust Mean: 49.9 ug/L
Std Dev: 10.4616 ug/L
Median: 49.5 ug/L

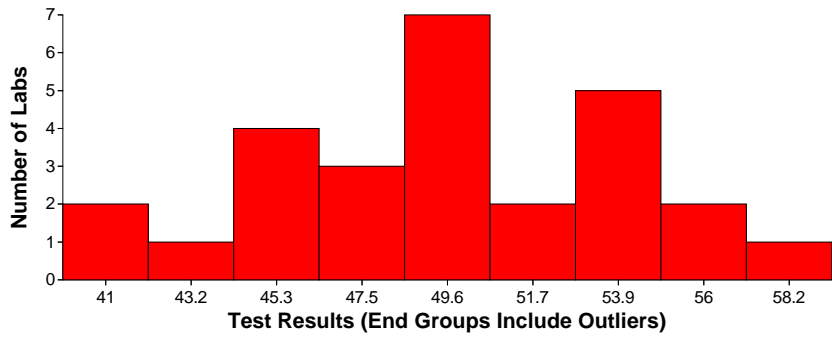

Totals for Matrix/Analyte/Technology:

Labs: Pass: 25 Fail: 2 Total: 27

Totals for Matrix/Analyte: Labs: Pass: 26 Fail: 2 Total: 28

Potable Water Methyl tert-butyl ether

Shipment: 407 Matrix: Potable Water
Analyte: Methyl tert-butyl ether
Sample: 0720
Technology: GC-PID
Prep Method:
Target: 47.2 ug/L
Limits: 37.8 to 56.6 ug/L
Basis: Fixed Percent (2)
Robust Mean: 47.6 ug/L
Std Dev: 0 ug/L
Median: 47.6 ug/L

A histogram is not displayed for Technology: GC-PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 26 Fail: 2 Total: 28

Potable Water Methoxychlor

Shipment: 407 Matrix: Potable Water
Analyte: Methoxychlor
Sample: 0707A
Technology: GC-ECD
Prep Method:
Target: 12.4 ug/L
Limits: 6.82 to 18 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 11.7 ug/L
Std Dev: 1.5984 ug/L
Median: 11.4 ug/L

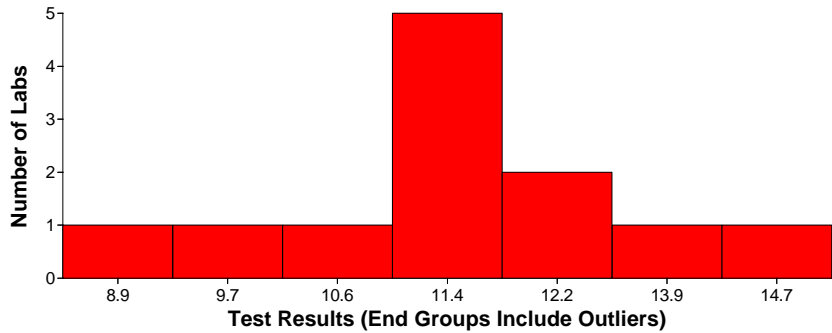


Totals for Matrix/Analyte/Technology:

Labs: Pass: 12 Fail: 0 Total: 12

Totals for Matrix/Analyte: Labs: Pass: 19 Fail: 0 Total: 19

Potable Water Methoxychlor

Shipment: 407 Matrix: Potable Water
Analyte: Methoxychlor
Sample: 0707A
Technology: GC-MS
Prep Method:
Target: 12.4 ug/L
Limits: 6.82 to 18 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 11 ug/L
Std Dev: 2.205 ug/L
Median: 11.3 ug/L

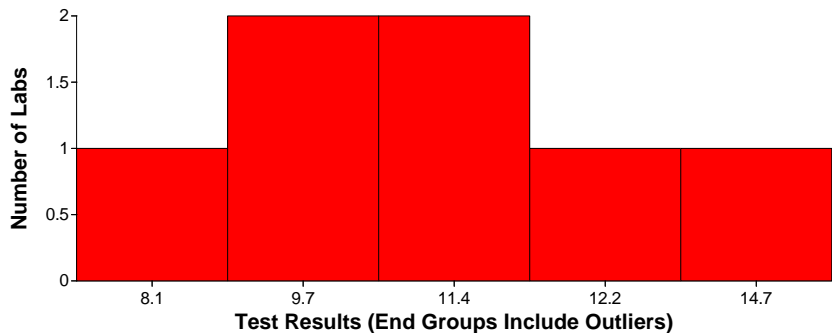

Totals for Matrix/Analyte/Technology:


Labs: Pass: 7 Fail: 0 Total: 7

Totals for Matrix/Analyte: Labs: Pass: 19 Fail: 0 Total: 19

Potable Water Sodium, Total

Potable Water Sodium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Sodium, Total
Sample: 0732
Technology: FAAS
Prep Method:
Target: 39.7 mg/L
Limits: 33.7 to 45.7 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 39.4 mg/L
Std Dev: 14.9172 mg/L
Median: 39.3 mg/L

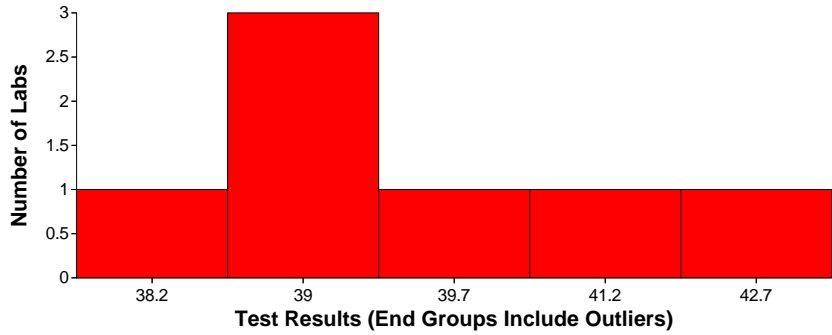

Totals for Matrix/Analyte/Technology:

Labs: Pass: 6 Fail: 1 Total: 7

Totals for Matrix/Analyte: Labs: Pass: 40 Fail: 1 Total: 41

Potable Water Sodium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Sodium, Total
Sample: 0732
Technology: IC
Prep Method:
Target: 39.7 mg/L
Limits: 33.7 to 45.7 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 37.6 mg/L
Std Dev: 0 mg/L
Median: 37.6 mg/L

A histogram is not displayed for Technology: IC due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 40 Fail: 1 Total: 41

Potable Water Sodium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Sodium, Total
Sample: 0732
Technology: ICP-AES
Prep Method:
Target: 39.7 mg/L
Limits: 33.7 to 45.7 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 39.8 mg/L
Std Dev: 7.1888 mg/L
Median: 40.05 mg/L

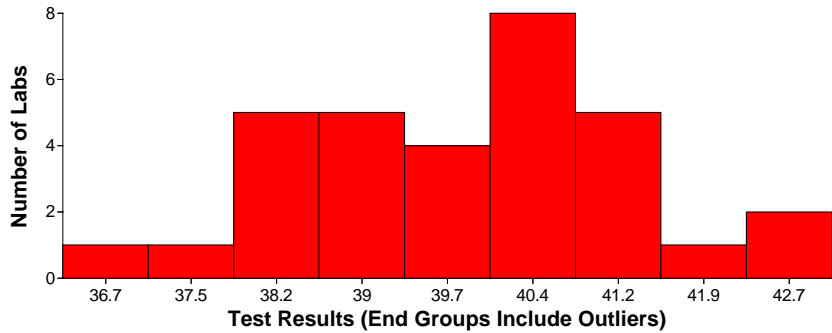

Totals for Matrix/Analyte/Technology:

Labs: Pass: 32 Fail: 0 Total: 32

Totals for Matrix/Analyte: Labs: Pass: 40 Fail: 1 Total: 41

Potable Water Sodium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Sodium, Total
Sample: 0732
Technology: ICP-MS
Prep Method:
Target: 39.7 mg/L
Limits: 33.7 to 45.7 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 41.6 mg/L
Std Dev: 0 mg/L
Median: 41.6 mg/L

A histogram is not displayed for Technology: ICP-MS due to the limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 40 Fail: 1 Total: 41

Potable Water Naphthalene

Potable Water Naphthalene


Shipment: 407 **Matrix:** Potable Water
Analyte: Naphthalene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 44.4 ug/L
Limits: 31.1 to 57.7 ug/L
Basis: Fixed Percent (2)
Robust Mean: 45.8 ug/L
Std Dev: 11.04 ug/L
Median: 45.1 ug/L

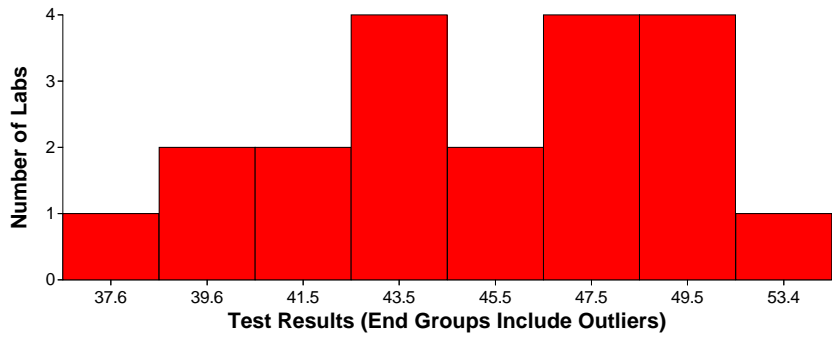

Totals for Matrix/Analyte/Technology:
Labs: Pass: 19 **Fail:** 1 **Total:** 20
Totals for Matrix/Analyte: **Labs: Pass:** 19 **Fail:** 1 **Total:** 20

Potable Water n-Butylbenzene

Shipment: 407 **Matrix:** Potable Water
Analyte: n-Butylbenzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 17 ug/L
Limits: 13.6 to 20.4 ug/L
Basis: Fixed Percent (2)
Robust Mean: 16.3 ug/L
Std Dev: 3.2874 ug/L
Median: 16.3 ug/L

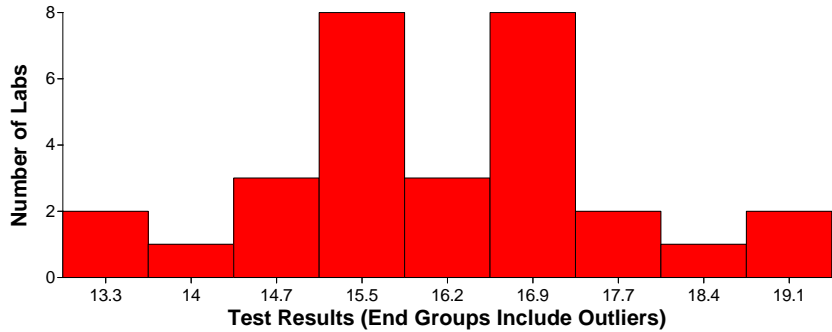

Totals for Matrix/Analyte/Technology:
Labs: Pass: 28 **Fail:** 2 **Total:** 30
Totals for Matrix/Analyte: **Labs: Pass:** 29 **Fail:** 2 **Total:** 31

Potable Water n-Butylbenzene


Shipment: 407 **Matrix:** Potable Water
Analyte: n-Butylbenzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 17 ug/L
Limits: 13.6 to 20.4 ug/L
Basis: Fixed Percent (2)
Robust Mean: 14.7 ug/L
Std Dev: 0 ug/L
Median: 14.7 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
Labs: Pass: 1 **Fail:** 0 **Total:** 1
Totals for Matrix/Analyte: **Labs: Pass:** 29 **Fail:** 2 **Total:** 31

Potable Water Nickel, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Nickel, Total
Sample: 0706
Technology: FAAS
Prep Method:
Target: 25 ug/L
Limits: 21.3 to 28.8 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 21 ug/L
Std Dev: 12.1244 ug/L
Median: 31 ug/L

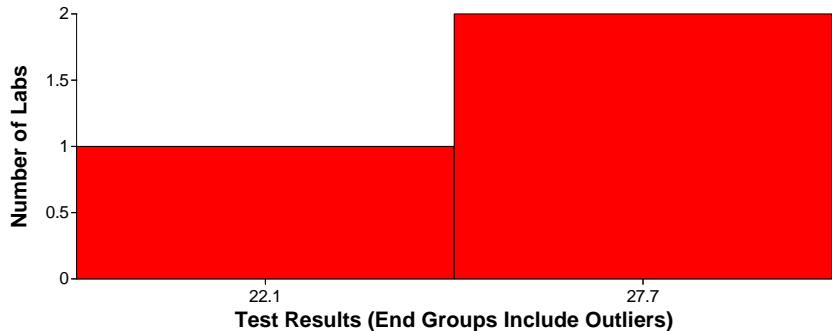


Totals for Matrix/Analyte/Technology:
Labs: Pass: 0 **Fail:** 3 **Total:** 3
Totals for Matrix/Analyte: **Labs: Pass:** 47 **Fail:** 8 **Total:** 55

Potable Water Nickel, Total

Potable Water Nickel, Total


Shipment: 407 Matrix: Potable Water
 Analyte: Nickel, Total
 Sample: 0706
 Technology: ICP-AES
 Prep Method:
 Target: 25 ug/L
 Limits: 21.3 to 28.8 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 25.4 ug/L
 Std Dev: 7.4219 ug/L
 Median: 25 ug/L

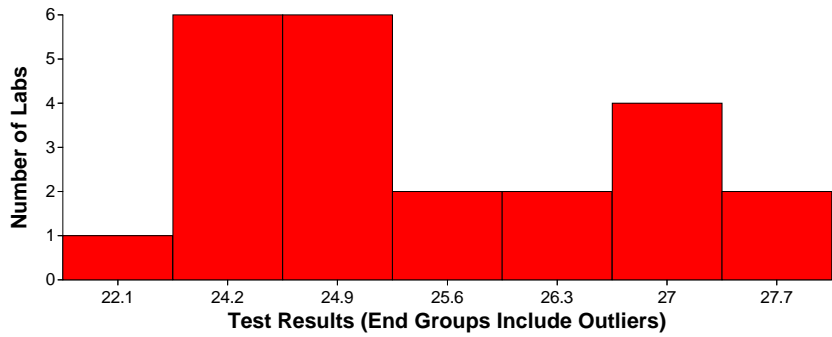

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 20 Fail: 3 Total: 23
 Totals for Matrix/Analyte: Labs: Pass: 47 Fail: 8 Total: 55

Potable Water Nickel, Total


Shipment: 407 Matrix: Potable Water
 Analyte: Nickel, Total
 Sample: 0706
 Technology: ICP-MS
 Prep Method:
 Target: 25 ug/L
 Limits: 21.3 to 28.8 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 24.6 ug/L
 Std Dev: 6.455 ug/L
 Median: 24.5 ug/L

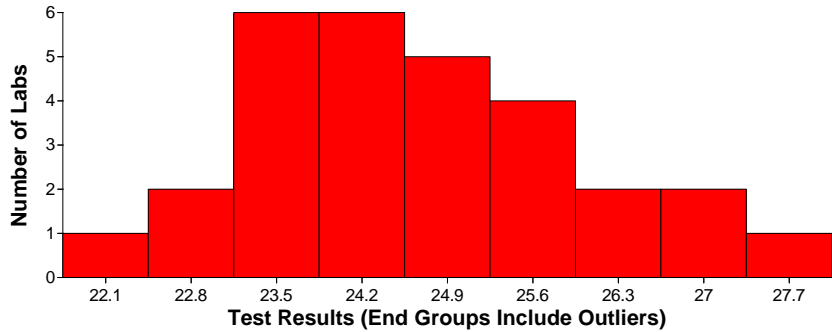

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 27 Fail: 2 Total: 29
 Totals for Matrix/Analyte: Labs: Pass: 47 Fail: 8 Total: 55

Potable Water Nitrite (as N)


Shipment: 407 Matrix: Potable Water
 Analyte: Nitrite (as N)
 Sample: 0727
 Technology: AUTO
 Prep Method:
 Target: 1.69 mg/L
 Limits: 1.44 to 1.94 mg/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 1.7 mg/L
 Std Dev: 0.0518 mg/L
 Median: 1.71 mg/L

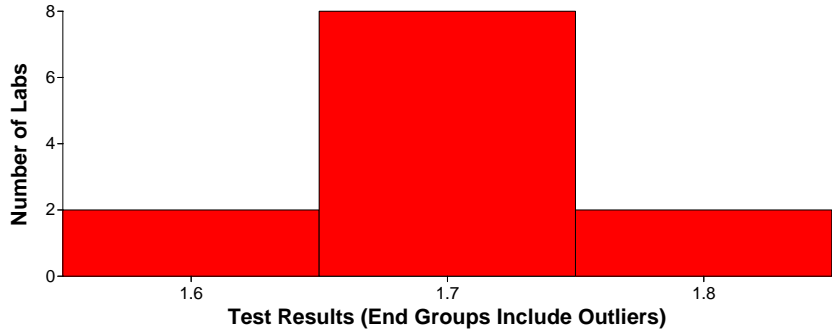

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 12 Fail: 0 Total: 12
 Totals for Matrix/Analyte: Labs: Pass: 48 Fail: 4 Total: 52

Potable Water Nitrite (as N)

Shipment: 407 Matrix: Potable Water
 Analyte: Nitrite (as N)
 Sample: 0727
 Technology: COLOR
 Prep Method:
 Target: 1.69 mg/L
 Limits: 1.44 to 1.94 mg/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 1.7 mg/L
 Std Dev: 0.4 mg/L
 Median: 1.72 mg/L

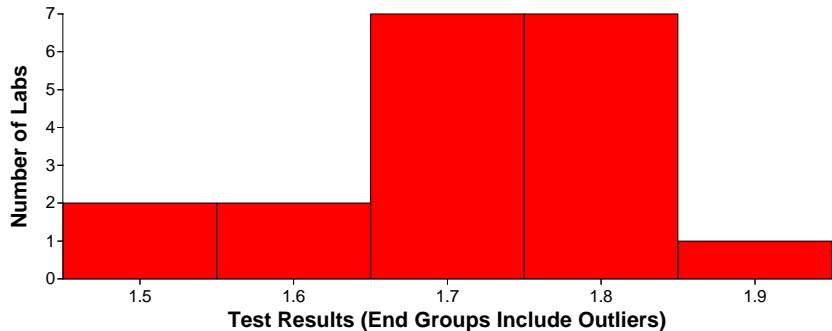


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 18 Fail: 1 Total: 19
 Totals for Matrix/Analyte: Labs: Pass: 48 Fail: 4 Total: 52

Potable Water Nitrite (as N)

Potable Water Nitrite (as N)

Shipment: 407 Matrix: Potable Water
Analyte: Nitrite (as N)
Sample: 0727
Technology: IC-COND
Prep Method:
Target: 1.69 mg/L
Limits: 1.44 to 1.94 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 1.7 mg/L
Std Dev: 0.525 mg/L
Median: 1.73 mg/L

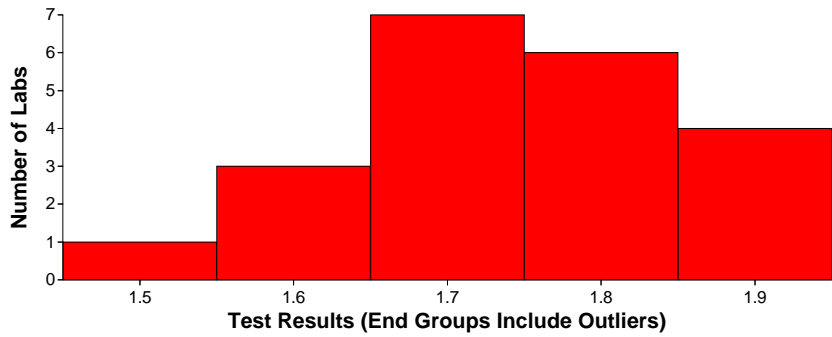


Totals for Matrix/Analyte/Technology:

Labs: Pass: 18 Fail: 3 Total: 21

Totals for Matrix/Analyte: Labs: Pass: 48 Fail: 4 Total: 52

Potable Water Nitrate (as N)

Shipment: 407 Matrix: Potable Water
Analyte: Nitrate (as N)
Sample: 0702
Technology: AUTO
Prep Method:
Target: 8.05 mg/L
Limits: 7.25 to 8.86 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 8 mg/L
Std Dev: 0.352 mg/L
Median: 8.05 mg/L

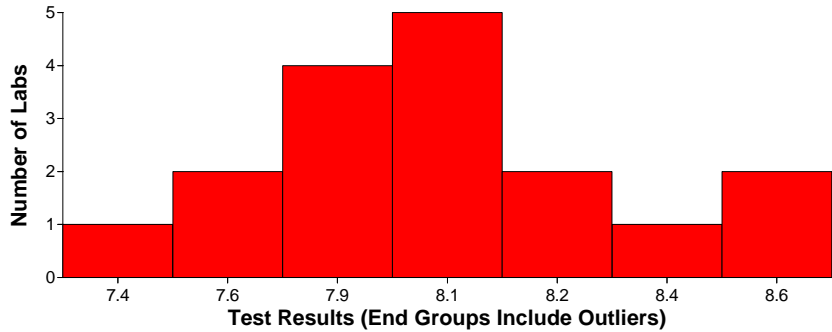


Totals for Matrix/Analyte/Technology:

Labs: Pass: 16 Fail: 1 Total: 17

Totals for Matrix/Analyte: Labs: Pass: 60 Fail: 2 Total: 62

Potable Water Nitrate (as N)

Shipment: 407 Matrix: Potable Water
Analyte: Nitrate (as N)
Sample: 0702
Technology: COLOR
Prep Method:
Target: 8.05 mg/L
Limits: 7.25 to 8.86 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 8.1 mg/L
Std Dev: 0.258 mg/L
Median: 7.99 mg/L

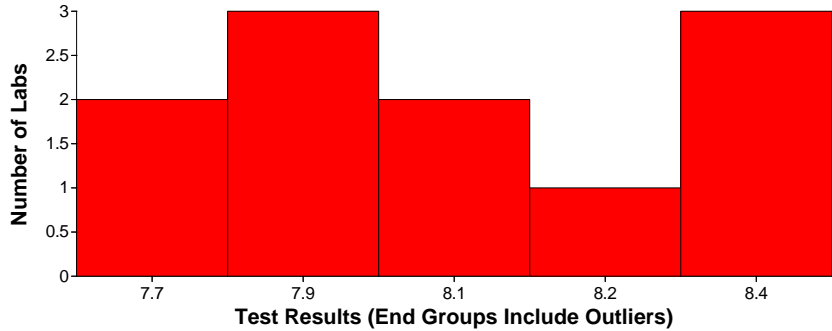


Totals for Matrix/Analyte/Technology:

Labs: Pass: 11 Fail: 0 Total: 11

Totals for Matrix/Analyte: Labs: Pass: 60 Fail: 2 Total: 62

Potable Water Nitrate (as N)

Shipment: 407 Matrix: Potable Water
Analyte: Nitrate (as N)
Sample: 0702
Technology: IC-COND
Prep Method:
Target: 8.05 mg/L
Limits: 7.25 to 8.86 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 8.1 mg/L
Std Dev: 0.3383 mg/L
Median: 8.05 mg/L

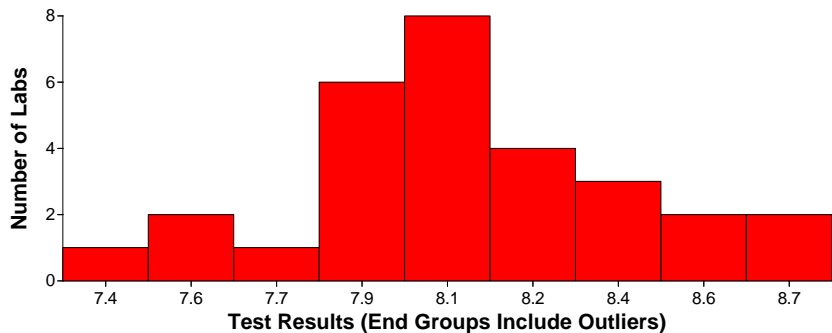

Totals for Matrix/Analyte/Technology:


Labs: Pass: 29 Fail: 0 Total: 29

Totals for Matrix/Analyte: Labs: Pass: 60 Fail: 2 Total: 62

Potable Water Nitrate (as N)

Potable Water Nitrate (as N)

Shipment: 407 Matrix: Potable Water
Analyte: Nitrate (as N)
Sample: 0702
Technology: POT
Prep Method:
Target: 8.05 mg/L
Limits: 7.25 to 8.86 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 8.2 mg/L
Std Dev: 3.6814 mg/L
Median: 8 mg/L

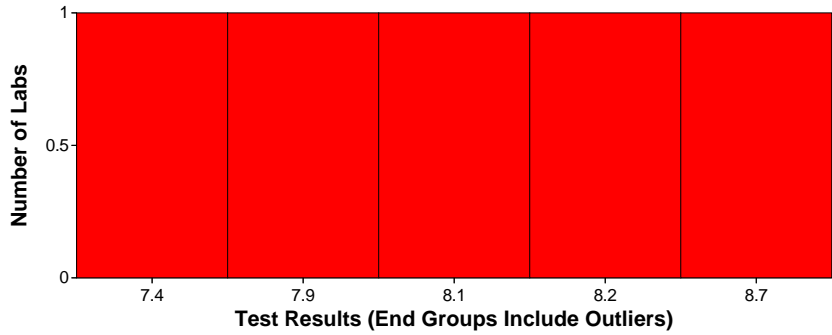


Totals for Matrix/Analyte/Technology:

Labs: Pass: 4 Fail: 1 Total: 5

Totals for Matrix/Analyte: Labs: Pass: 60 Fail: 2 Total: 62

Potable Water n-Propylbenzene

Shipment: 407 Matrix: Potable Water
Analyte: n-Propylbenzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 12.9 ug/L
Limits: 10.3 to 15.5 ug/L
Basis: Fixed Percent (2)
Robust Mean: 12.9 ug/L
Std Dev: 3.408 ug/L
Median: 12.9 ug/L

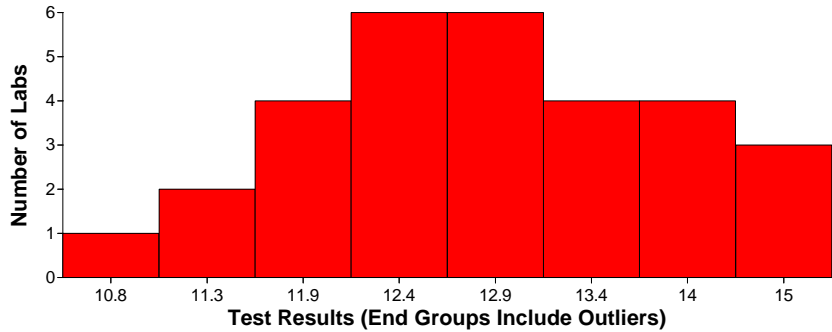

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 2 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water n-Propylbenzene

Shipment: 407 Matrix: Potable Water
Analyte: n-Propylbenzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 12.9 ug/L
Limits: 10.3 to 15.5 ug/L
Basis: Fixed Percent (2)
Robust Mean: 11.8 ug/L
Std Dev: 0 ug/L
Median: 11.8 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water Aldicarb Sulfoxide

Shipment: 407 Matrix: Potable Water
Analyte: Aldicarb Sulfoxide
Sample: 0715
Technology: HPLC-FLUOR
Prep Method:
Target: 37.7 ug/L
Limits: 28.3 to 47.1 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 37 ug/L
Std Dev: 2.3913 ug/L
Median: 36.72 ug/L

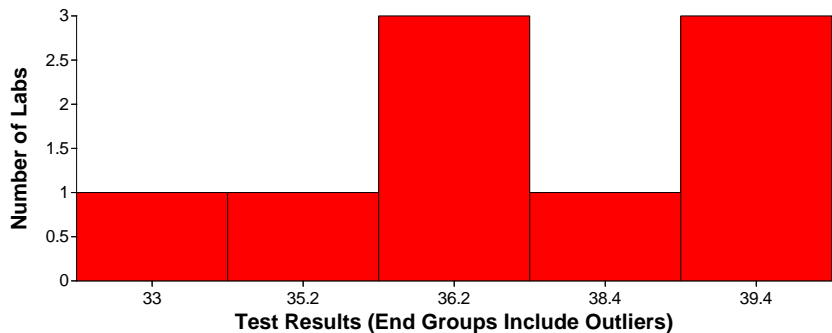

Totals for Matrix/Analyte/Technology:

Labs: Pass: 9 Fail: 0 Total: 9


Totals for Matrix/Analyte: Labs: Pass: 9 Fail: 0 Total: 9

Potable Water Lead, Total

Potable Water Lead, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Lead, Total
 Sample: 0706
 Technology: GFAAS
 Prep Method:
 Target: 96.2 ug/L
 Limits: 67.3 to 125 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 95.2 ug/L
 Std Dev: 21.3581 ug/L
 Median: 95.1 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 21 Fail: 0 Total: 21
 Totals for Matrix/Analyte: Labs: Pass: 55 Fail: 3 Total: 58

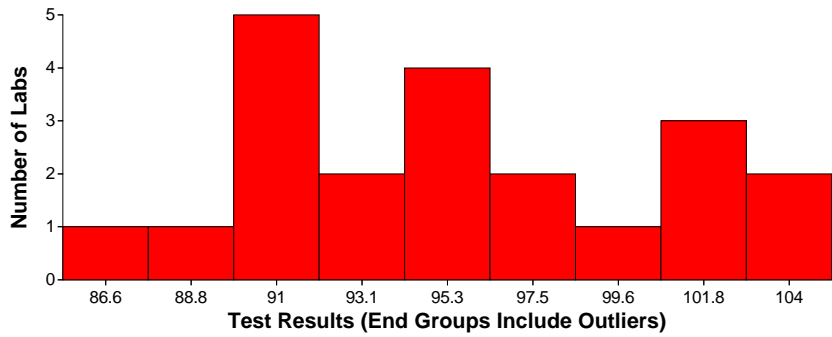

Potable Water Lead, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Lead, Total
 Sample: 0706
 Technology: ICP-AES
 Prep Method:
 Target: 96.2 ug/L
 Limits: 67.3 to 125 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 95.6 ug/L
 Std Dev: 52.3673 ug/L
 Median: 96.7 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 4 Fail: 2 Total: 6
 Totals for Matrix/Analyte: Labs: Pass: 55 Fail: 3 Total: 58

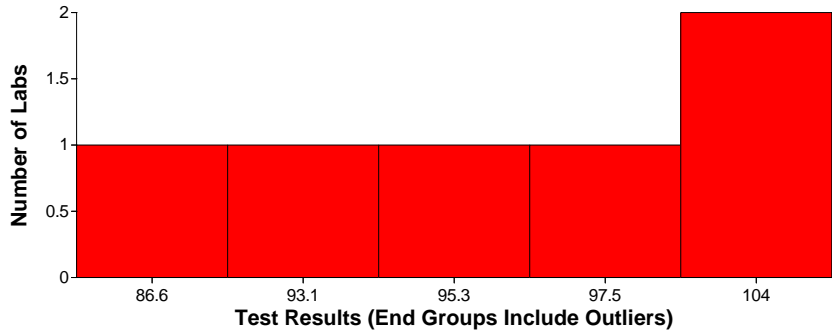

Potable Water Lead, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Lead, Total
 Sample: 0706
 Technology: ICP-MS
 Prep Method:
 Target: 96.2 ug/L
 Limits: 67.3 to 125 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 95.1 ug/L
 Std Dev: 17.4625 ug/L
 Median: 95.5 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 30 Fail: 1 Total: 31
 Totals for Matrix/Analyte: Labs: Pass: 55 Fail: 3 Total: 58

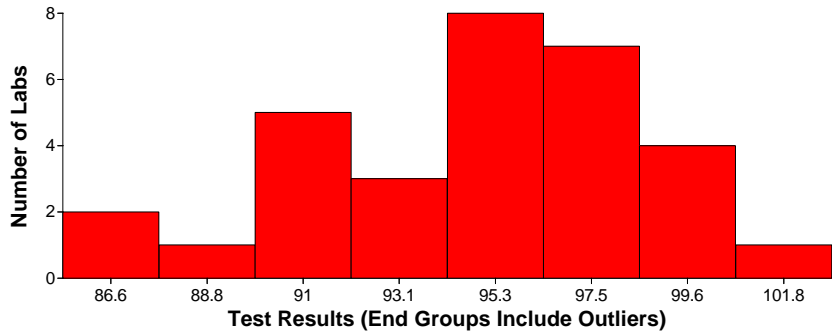

Potable Water PCB, Total (as decachlorobiphenyl)

Shipment: 407 Matrix: Potable Water
 Analyte: PCB, Total (as decachlorobiphenyl)
 Sample: 0725
 Technology: GC-ECD
 Prep Method:
 Target: 2.72 ug/L
 Limits: 0 to 5.44 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 3.5 ug/L
 Std Dev: 1.4508 ug/L
 Median: 2.7 ug/L


Totals for Matrix/Analyte/Technology:
 Labs: Pass: 3 Fail: 0 Total: 3
 Totals for Matrix/Analyte: Labs: Pass: 3 Fail: 0 Total: 3

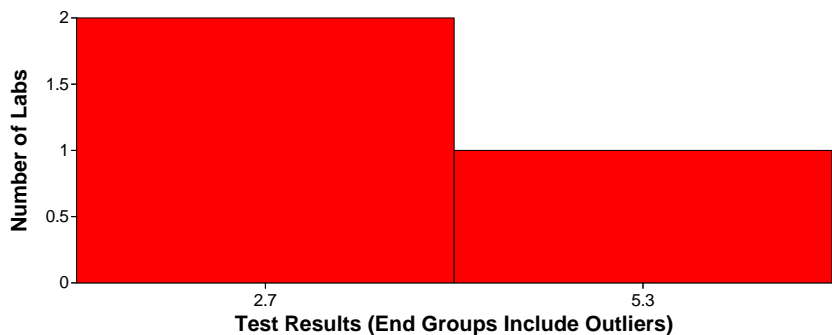

Potable Water Pentachlorophenol

Potable Water Pentachlorophenol

Shipment: 407 Matrix: Potable Water
Analyte: Pentachlorophenol
Sample: 0717
Technology: GC-ECD
Prep Method:
Target: 20.4 ug/L
Limits: 10.2 to 30.6 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 19 ug/L
Std Dev: 6.1184 ug/L
Median: 19.1 ug/L

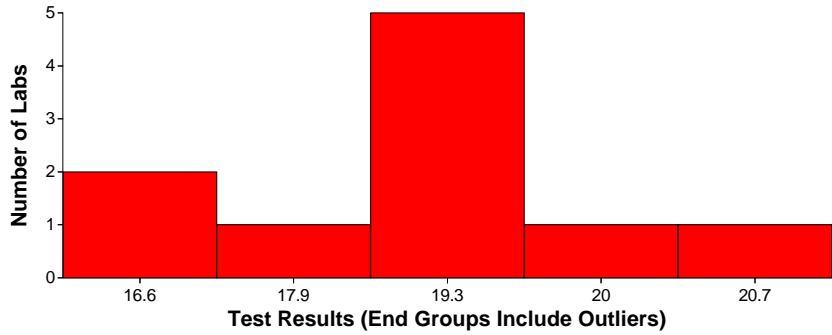

Totals for Matrix/Analyte/Technology:

Labs: Pass: 10 Fail: 0 Total: 10

Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water Pentachlorophenol

Shipment: 407 Matrix: Potable Water
Analyte: Pentachlorophenol
Sample: 0717
Technology: HPLC-UV
Prep Method:
Target: 20.4 ug/L
Limits: 10.2 to 30.6 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 21.3 ug/L
Std Dev: 0 ug/L
Median: 21.3 ug/L

A histogram is not displayed for Technology: HPLC-UV due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water p-Isopropyltoluene (P-Cymene)

Shipment: 407 Matrix: Potable Water
Analyte: p-Isopropyltoluene (P-Cymene)
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 17.3 ug/L
Limits: 13.8 to 20.8 ug/L
Basis: Fixed Percent (2)
Robust Mean: 17.6 ug/L
Std Dev: 3.4705 ug/L
Median: 17.55 ug/L

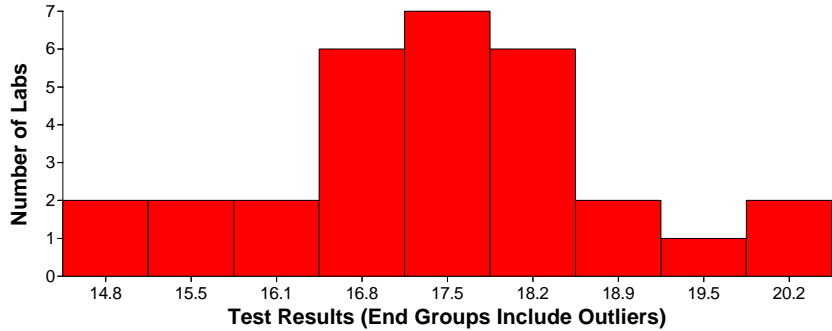

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water p-Isopropyltoluene (P-Cymene)

Shipment: 407 Matrix: Potable Water
Analyte: p-Isopropyltoluene (P-Cymene)
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 17.3 ug/L
Limits: 13.8 to 20.8 ug/L
Basis: Fixed Percent (2)
Robust Mean: 15.4 ug/L
Std Dev: 0 ug/L
Median: 15.4 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water Perchlorate

Shipment: 407 Matrix: Potable Water
Analyte: Perchlorate
Sample: 0737
Technology: HPLC-ESMS
Prep Method:
Target: 11.3 ug/L
Limits: 9.04 to 13.6 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 11.2 ug/L
Std Dev: 0 ug/L
Median: 11.2 ug/L

A histogram is not displayed for
Technology: HPLC-ESMS due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 4 Fail: 0 Total: 4

Potable Water Perchlorate

Shipment: 407 Matrix: Potable Water
Analyte: Perchlorate
Sample: 0737
Technology: IC-COND
Prep Method:
Target: 11.3 ug/L
Limits: 9.04 to 13.6 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 10.2 ug/L
Std Dev: 0.895 ug/L
Median: 10.21 ug/L

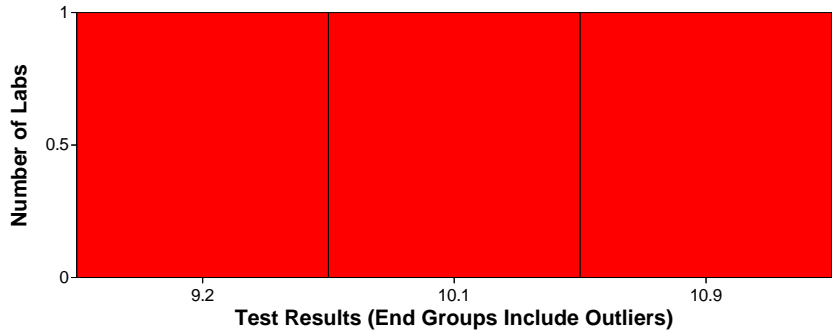


Totals for Matrix/Analyte/Technology:

Labs: Pass: 3 Fail: 0 Total: 3

Totals for Matrix/Analyte: Labs: Pass: 4 Fail: 0 Total: 4

Potable Water Picloram

Shipment: 407 Matrix: Potable Water
Analyte: Picloram
Sample: 0717
Technology: GC-ECD
Prep Method:
Target: 76.8 ug/L
Limits: 38.4 to 115 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 72 ug/L
Std Dev: 17.6175 ug/L
Median: 71.1 ug/L

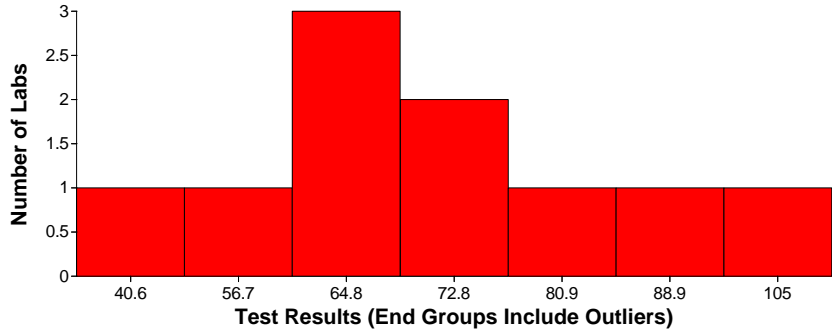

Totals for Matrix/Analyte/Technology:

Labs: Pass: 10 Fail: 0 Total: 10

Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water Picloram

Shipment: 407 Matrix: Potable Water
Analyte: Picloram
Sample: 0717
Technology: HPLC-UV
Prep Method:
Target: 76.8 ug/L
Limits: 38.4 to 115 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 79.5 ug/L
Std Dev: 0 ug/L
Median: 79.5 ug/L

A histogram is not displayed for
Technology: HPLC-UV due to the
limited number of participants.

Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water Orthophosphate (as P)

Potable Water Orthophosphate (as P)

Shipment: 407 **Matrix:** Potable Water
Analyte: Orthophosphate (as P)
Sample: 0702
Technology: AUTO
Prep Method:
Target: 2.34 mg/L
Limits: 1.99 to 2.69 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 2.3 mg/L
Std Dev: 0.0566 mg/L
Median: 2.28 mg/L

A histogram is not displayed for Technology: AUTO due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 2 Fail: 0 Total: 2

Totals for Matrix/Analyte: Labs: Pass: 40 Fail: 2 Total: 42

Potable Water Orthophosphate (as P)

Shipment: 407 **Matrix:** Potable Water
Analyte: Orthophosphate (as P)
Sample: 0702
Technology: COLOR
Prep Method:
Target: 2.34 mg/L
Limits: 1.99 to 2.69 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 2.4 mg/L
Std Dev: 0.6999 mg/L
Median: 2.32 mg/L

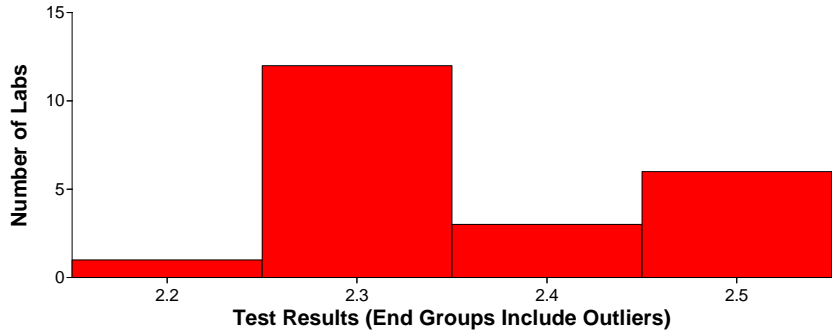


Totals for Matrix/Analyte/Technology:

Labs: Pass: 21 Fail: 1 Total: 22

Totals for Matrix/Analyte: Labs: Pass: 40 Fail: 2 Total: 42

Potable Water Orthophosphate (as P)

Shipment: 407 **Matrix:** Potable Water
Analyte: Orthophosphate (as P)
Sample: 0702
Technology: IC-COND
Prep Method:
Target: 2.34 mg/L
Limits: 1.99 to 2.69 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 2.3 mg/L
Std Dev: 0.5396 mg/L
Median: 2.28 mg/L

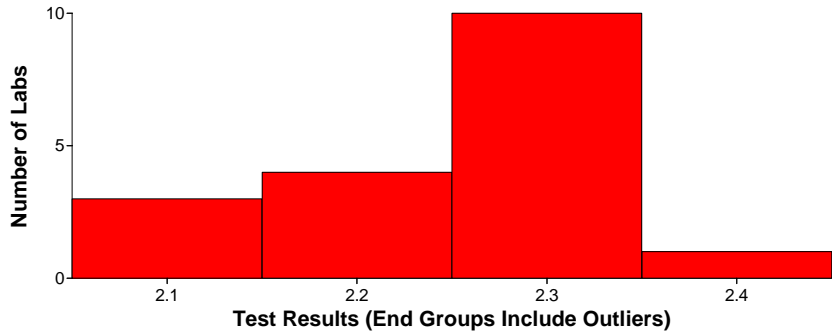


Totals for Matrix/Analyte/Technology:

Labs: Pass: 17 Fail: 1 Total: 18

Totals for Matrix/Analyte: Labs: Pass: 40 Fail: 2 Total: 42

Potable Water Propachlor

Shipment: 407 **Matrix:** Potable Water
Analyte: Propachlor
Sample: 0707A
Technology: GC-ECD
Prep Method:
Target: 1.32 ug/L
Limits: 0.726 to 1.91 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 1.1 ug/L
Std Dev: 0.0772 ug/L
Median: 1.14 ug/L

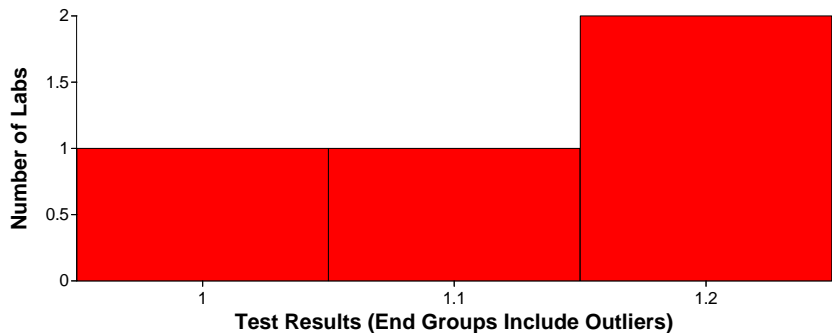

Totals for Matrix/Analyte/Technology:

Labs: Pass: 4 Fail: 0 Total: 4

Totals for Matrix/Analyte: Labs: Pass: 15 Fail: 0 Total: 15

Potable Water Propachlor

Potable Water Propachlor

Shipment: 407 Matrix: Potable Water

Analyte: Propachlor

Sample: 0707A

Technology: GC-MS

Prep Method:

Target: 1.32 ug/L

Limits: 0.726 to 1.91 ug/L

Basis: Target Value +/- a fixed percent

Robust Mean: 1.3 ug/L


Std Dev: 0.146 ug/L

Median: 1.34 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 11 Fail: 0 Total: 11

Totals for Matrix/Analyte: Labs: Pass: 15 Fail: 0 Total: 15

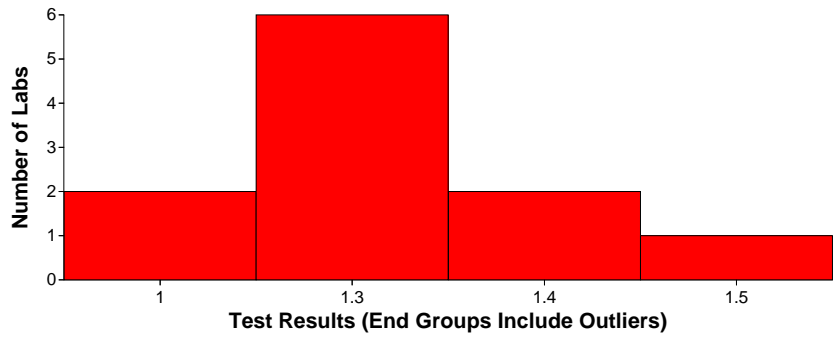

Potable Water Solids, Total Dissolved

Shipment: 407 Matrix: Potable Water

Analyte: Solids, Total Dissolved

Sample: 0731

Technology: GRAV

Prep Method:

Target: 584 mg/L

Limits: 467 to 701 mg/L

Basis: Target Value +/- a fixed percent

Robust Mean: 574.7 mg/L


Std Dev: 92.3522 mg/L

Median: 577 mg/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 41 Fail: 0 Total: 41

Totals for Matrix/Analyte: Labs: Pass: 41 Fail: 0 Total: 41

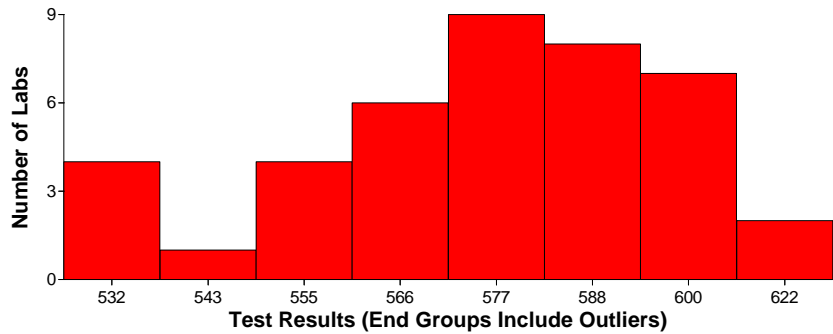

Potable Water Antimony, Total

Shipment: 407 Matrix: Potable Water

Analyte: Antimony, Total

Sample: 0706

Technology: GFAAS

Prep Method:

Target: 31.3 ug/L

Limits: 21.9 to 40.7 ug/L

Basis: Target Value +/- a fixed percent

Robust Mean: 32.5 ug/L


Std Dev: 10.9356 ug/L

Median: 31.7 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 9 Fail: 0 Total: 9

Totals for Matrix/Analyte: Labs: Pass: 38 Fail: 1 Total: 39

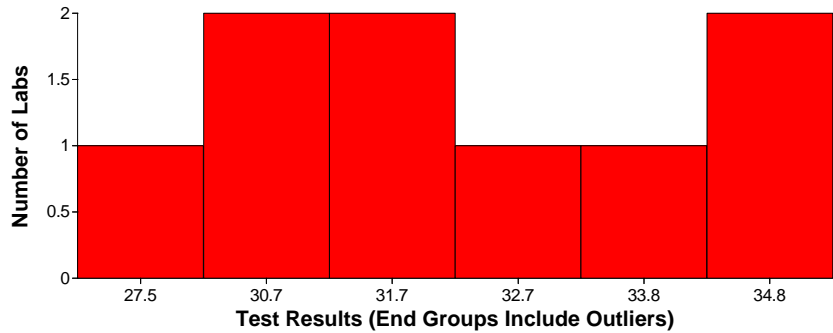

Potable Water Antimony, Total

Shipment: 407 Matrix: Potable Water

Analyte: Antimony, Total

Sample: 0706

Technology: ICP-AES

Prep Method:

Target: 31.3 ug/L

Limits: 21.9 to 40.7 ug/L

Basis: Target Value +/- a fixed percent

Robust Mean: 34.1 ug/L

Std Dev: 2.3335 ug/L

Median: 34.05 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 2 Fail: 0 Total: 2


Totals for Matrix/Analyte: Labs: Pass: 38 Fail: 1 Total: 39

A histogram is not displayed for Technology: ICP-AES due to the limited number of participants.

Potable Water Antimony, Total

Potable Water Antimony, Total

Shipment: 407 Matrix: Potable Water
Analyte: Antimony, Total
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 31.3 ug/L
Limits: 21.9 to 40.7 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 31.3 ug/L
Std Dev: 6.2106 ug/L
Median: 31.45 ug/L

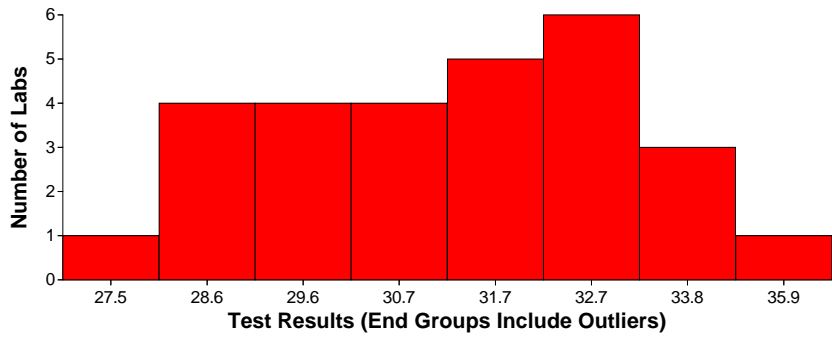


Totals for Matrix/Analyte/Technology:

Labs: Pass: 27 Fail: 1 Total: 28

Totals for Matrix/Analyte: Labs: Pass: 38 Fail: 1 Total: 39

Potable Water sec-Butylbenzene

Shipment: 407 Matrix: Potable Water
Analyte: sec-Butylbenzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 18.2 ug/L
Limits: 14.6 to 21.8 ug/L
Basis: Fixed Percent (2)
Robust Mean: 17.9 ug/L
Std Dev: 4.7129 ug/L
Median: 18.15 ug/L

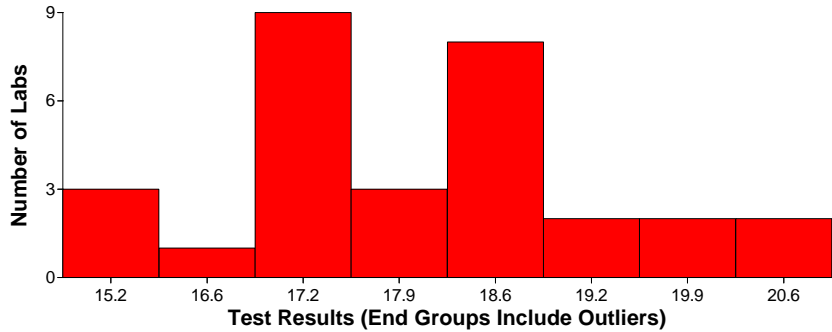

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 2 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water sec-Butylbenzene

Shipment: 407 Matrix: Potable Water
Analyte: sec-Butylbenzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 18.2 ug/L
Limits: 14.6 to 21.8 ug/L
Basis: Fixed Percent (2)
Robust Mean: 15.3 ug/L
Std Dev: 0 ug/L
Median: 15.3 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water Specific Conductance

Shipment: 407 Matrix: Potable Water
Analyte: Specific Conductance
Sample: 0724
Technology: COND
Prep Method:
Target: 362 umhos/cm
Limits: 326 to 398 umhos/cm
Basis: Target Value +/- a fixed percent
Robust Mean: 364.8 umhos/cm
Std Dev: 11.8447 umhos/cm
Median: 364 umhos/cm

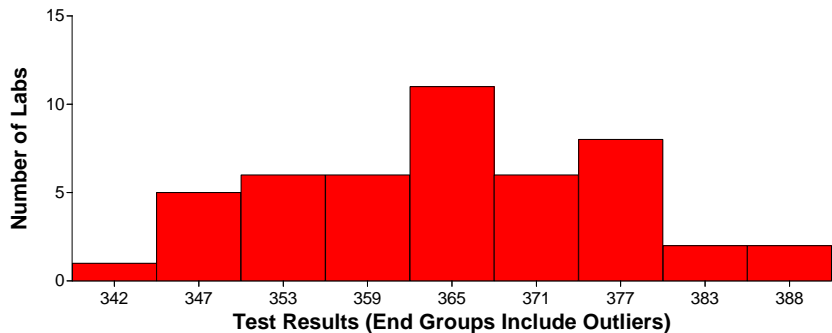

Totals for Matrix/Analyte/Technology:

Labs: Pass: 47 Fail: 0 Total: 47

Totals for Matrix/Analyte: Labs: Pass: 47 Fail: 0 Total: 47

Potable Water Selenium, Total


Potable Water Selenium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Selenium, Total
Sample: 0706
Technology: GFAAS
Prep Method:
Target: 22.5 ug/L
Limits: 18 to 27 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 21.8 ug/L
Std Dev: 1.0513 ug/L
Median: 21.6 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 9 Fail: 0 Total: 9

Totals for Matrix/Analyte: Labs: Pass: 37 Fail: 3 Total: 40

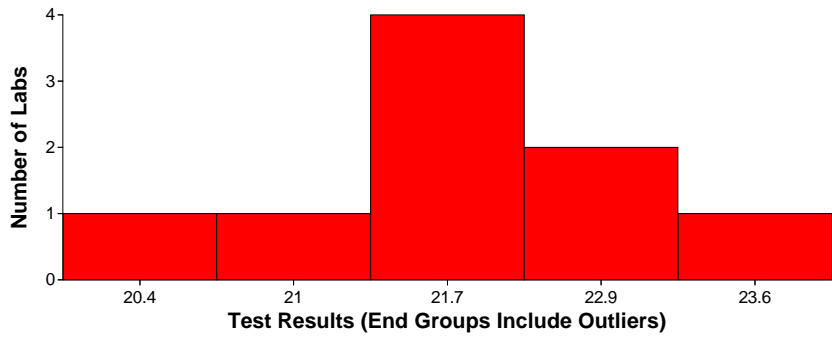

Potable Water Selenium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Selenium, Total
Sample: 0706
Technology: ICP-AES
Prep Method:
Target: 22.5 ug/L
Limits: 18 to 27 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 23.2 ug/L
Std Dev: 16.4049 ug/L
Median: 15.1 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 1 Total: 2

Totals for Matrix/Analyte: Labs: Pass: 37 Fail: 3 Total: 40

A histogram is not displayed for Technology: ICP-AES due to the limited number of participants.


Potable Water Selenium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Selenium, Total
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 22.5 ug/L
Limits: 18 to 27 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 22.2 ug/L
Std Dev: 6.9839 ug/L
Median: 22.4 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 27 Fail: 2 Total: 29

Totals for Matrix/Analyte: Labs: Pass: 37 Fail: 3 Total: 40

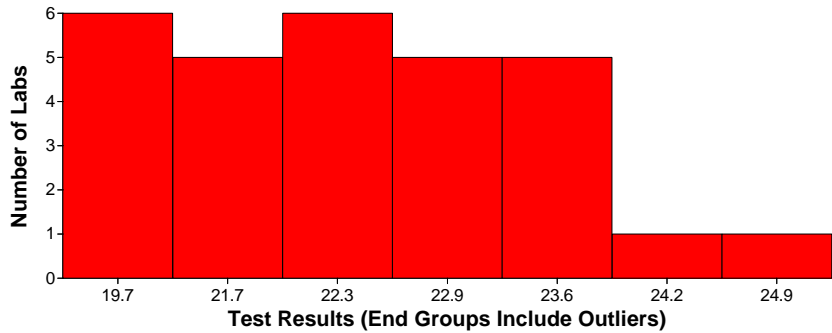

Potable Water Silica, Dissolved

Shipment: 407 Matrix: Potable Water
Analyte: Silica, Dissolved
Sample: 0728
Technology: AUTO
Prep Method:
Target: 47.4 mg/L
Limits: 40.3 to 54.5 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 53 mg/L
Std Dev: 0 mg/L
Median: 53 mg/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1


Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 1 Total: 12

A histogram is not displayed for Technology: AUTO due to the limited number of participants.

Potable Water Silica, Dissolved

Potable Water Silica, Dissolved


Shipment: 407 **Matrix:** Potable Water
Analyte: Silica, Dissolved
Sample: 0728
Technology: COLOR
Prep Method:
Target: 47.4 mg/L
Limits: 40.3 to 54.5 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 48.1 mg/L
Std Dev: 27.7579 mg/L
Median: 49 mg/L

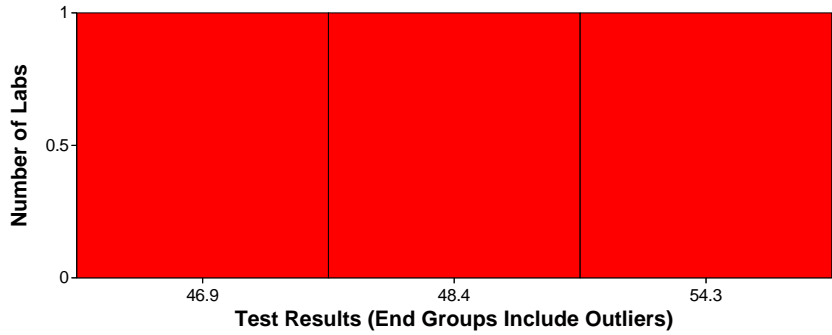

Totals for Matrix/Analyte/Technology:
Labs: Pass: 2 **Fail:** 1 **Total:** 3
Totals for Matrix/Analyte: **Labs: Pass:** 11 **Fail:** 1 **Total:** 12

Potable Water Silica, Dissolved


Shipment: 407 **Matrix:** Potable Water
Analyte: Silica, Dissolved
Sample: 0728
Technology: ICP-AES
Prep Method:
Target: 47.4 mg/L
Limits: 40.3 to 54.5 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 47.9 mg/L
Std Dev: 2.9645 mg/L
Median: 48.1 mg/L

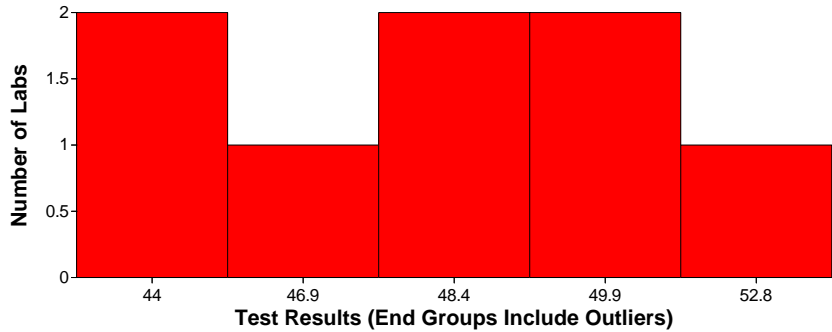

Totals for Matrix/Analyte/Technology:
Labs: Pass: 8 **Fail:** 0 **Total:** 8
Totals for Matrix/Analyte: **Labs: Pass:** 11 **Fail:** 1 **Total:** 12

Potable Water Simazine


Shipment: 407 **Matrix:** Potable Water
Analyte: Simazine
Sample: 0707B
Technology: GC-ECD
Prep Method:
Target: 5.33 ug/L
Limits: 2.93 to 7.73 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 6.2 ug/L
Std Dev: 0.9501 ug/L
Median: 6.68 ug/L

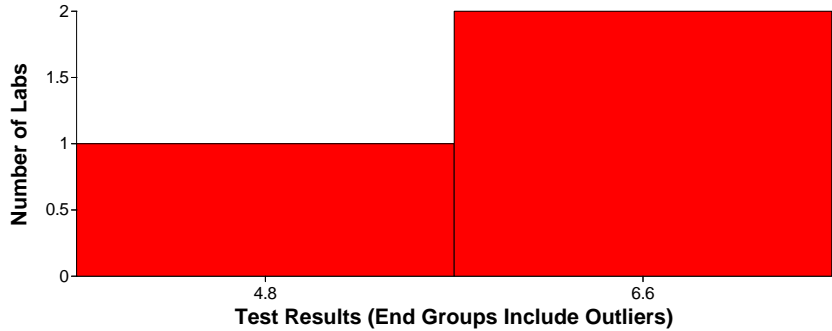

Totals for Matrix/Analyte/Technology:
Labs: Pass: 3 **Fail:** 0 **Total:** 3
Totals for Matrix/Analyte: **Labs: Pass:** 13 **Fail:** 1 **Total:** 14

Potable Water Simazine

Shipment: 407 **Matrix:** Potable Water
Analyte: Simazine
Sample: 0707B
Technology: GC-MS
Prep Method:
Target: 5.33 ug/L
Limits: 2.93 to 7.73 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 5.9 ug/L
Std Dev: 1.3724 ug/L
Median: 5.9 ug/L

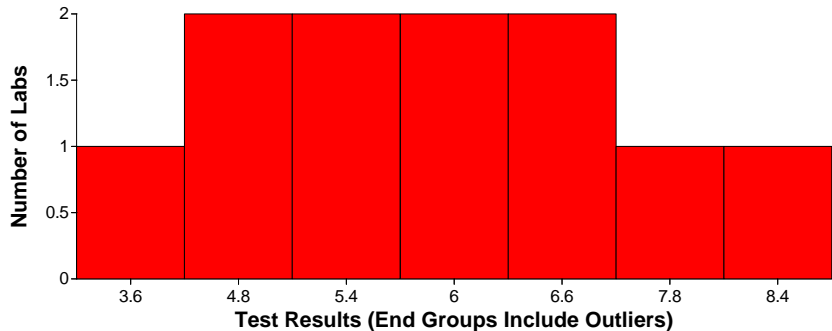


Totals for Matrix/Analyte/Technology:
Labs: Pass: 10 **Fail:** 1 **Total:** 11
Totals for Matrix/Analyte: **Labs: Pass:** 13 **Fail:** 1 **Total:** 14

Potable Water 2,4,5-TP (Silvex)

Potable Water 2,4,5-TP (Silvex)

Shipment: 407 Matrix: Potable Water
 Analyte: 2,4,5-TP (Silvex)
 Sample: 0717
 Technology: GC-ECD
 Prep Method:
 Target: 18.1 ug/L
 Limits: 9.05 to 27.2 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 16.7 ug/L
 Std Dev: 1.6057 ug/L
 Median: 16.6 ug/L

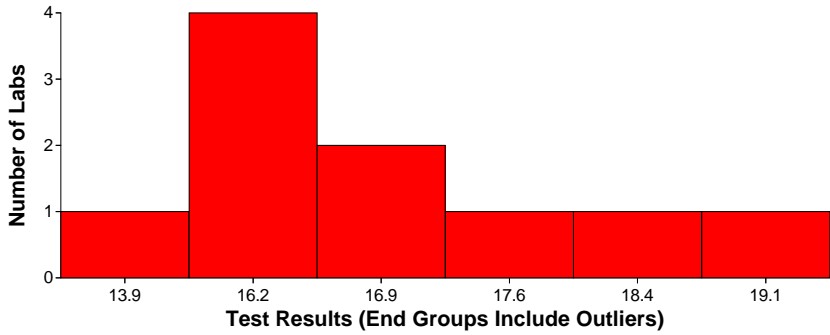

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 10 Fail: 0 Total: 10
 Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water 2,4,5-TP (Silvex)

Shipment: 407 Matrix: Potable Water
 Analyte: 2,4,5-TP (Silvex)
 Sample: 0717
 Technology: HPLC-UV
 Prep Method:
 Target: 18.1 ug/L
 Limits: 9.05 to 27.2 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 18 ug/L
 Std Dev: 0 ug/L
 Median: 18 ug/L

A histogram is not displayed for Technology: HPLC-UV due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 1 Fail: 0 Total: 1
 Totals for Matrix/Analyte: Labs: Pass: 11 Fail: 0 Total: 11

Potable Water Sulfate (as SO4)


Shipment: 407 Matrix: Potable Water
 Analyte: Sulfate (as SO4)
 Sample: 0702
 Technology: AUTO
 Prep Method:
 Target: 38 mg/L
 Limits: 32.3 to 43.7 mg/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 38.7 mg/L
 Std Dev: 0 mg/L
 Median: 38.7 mg/L

A histogram is not displayed for Technology: AUTO due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 1 Fail: 0 Total: 1
 Totals for Matrix/Analyte: Labs: Pass: 47 Fail: 2 Total: 49

Potable Water Sulfate (as SO4)

Shipment: 407 Matrix: Potable Water
 Analyte: Sulfate (as SO4)
 Sample: 0702
 Technology: COLOR
 Prep Method:
 Target: 38 mg/L
 Limits: 32.3 to 43.7 mg/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 37.6 mg/L
 Std Dev: 14.7987 mg/L
 Median: 38.3 mg/L

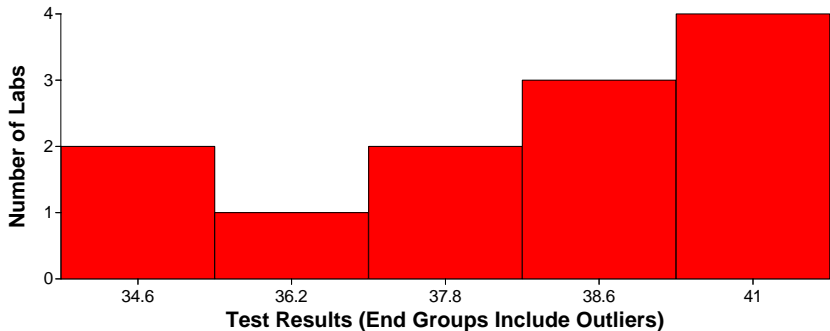

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 10 Fail: 2 Total: 12
 Totals for Matrix/Analyte: Labs: Pass: 47 Fail: 2 Total: 49

Potable Water Sulfate (as SO4)

Shipment: 407 Matrix: Potable Water
Analyte: Sulfate (as SO4)
Sample: 0702
Technology: GRAV
Prep Method:
Target: 38 mg/L
Limits: 32.3 to 43.7 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 38.7 mg/L
Std Dev: 0 mg/L
Median: 38.7 mg/L

A histogram is not displayed for
Technology: GRAV due to the
limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 47 Fail: 2 Total: 49

Potable Water Sulfate (as SO4)

Shipment: 407 Matrix: Potable Water
Analyte: Sulfate (as SO4)
Sample: 0702
Technology: IC-COND
Prep Method:
Target: 38 mg/L
Limits: 32.3 to 43.7 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 37.5 mg/L
Std Dev: 6.4978 mg/L
Median: 37.8 mg/L

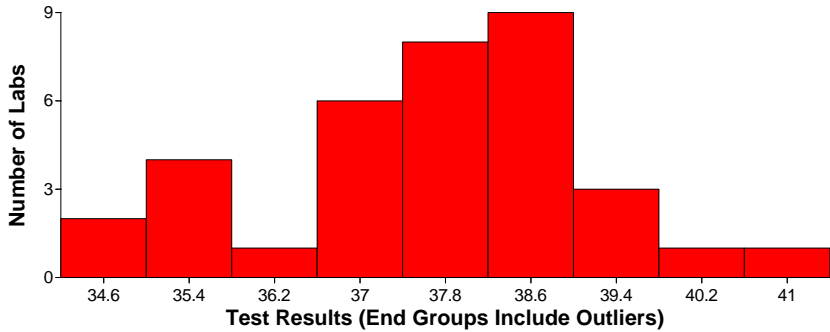


Totals for Matrix/Analyte/Technology:

Labs: Pass: 35 Fail: 0 Total: 35

Totals for Matrix/Analyte: Labs: Pass: 47 Fail: 2 Total: 49

Potable Water Styrene

Shipment: 407 Matrix: Potable Water
Analyte: Styrene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 15.1 ug/L
Limits: 12.1 to 18.1 ug/L
Basis: Fixed Percent (2)
Robust Mean: 14.9 ug/L
Std Dev: 3.0988 ug/L
Median: 14.875 ug/L

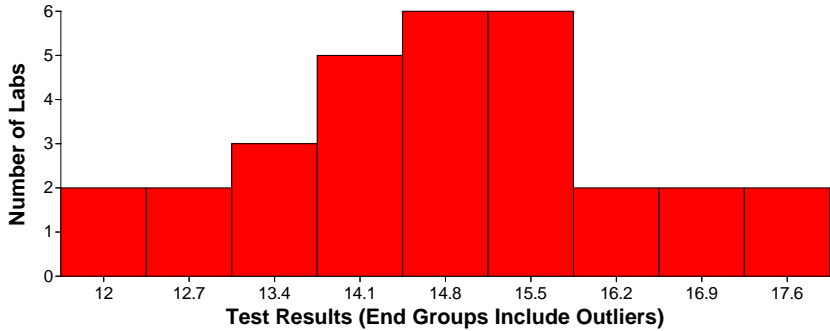

Totals for Matrix/Analyte/Technology:

Labs: Pass: 26 Fail: 4 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 27 Fail: 4 Total: 31

Potable Water Styrene

Shipment: 407 Matrix: Potable Water
Analyte: Styrene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 15.1 ug/L
Limits: 12.1 to 18.1 ug/L
Basis: Fixed Percent (2)
Robust Mean: 14.1 ug/L
Std Dev: 0 ug/L
Median: 14.1 ug/L

A histogram is not displayed for
Technology: GCELCD/PID due to the
limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 27 Fail: 4 Total: 31

Potable Water Surfactant (MBAS)

Potable Water Surfactant (MBAS)

Shipment: 407 **Matrix:** Potable Water
Analyte: Surfactant (MBAS)
Sample: 0736
Technology: COLOR
Prep Method:
Target: 0.805 mg/L
Limits: 0.617 to 0.973 mg/L
Basis: Linear Regression
Robust Mean: 0.9 mg/L
Std Dev: 0.1433 mg/L
Median: 0.87 mg/L

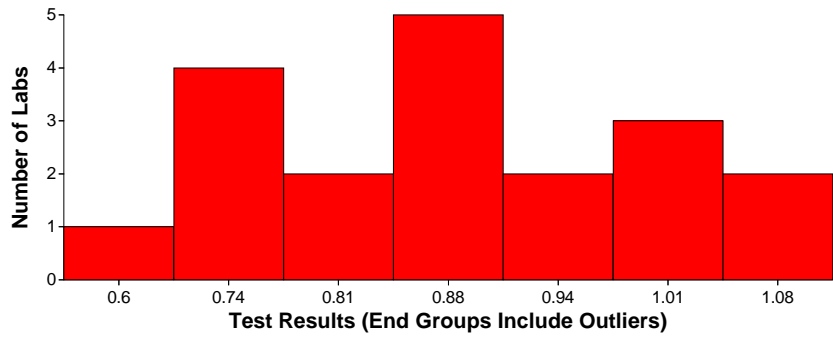


Totals for Matrix/Analyte/Technology:

Labs: Pass: 13 **Fail:** 6 **Total:** 19

Totals for Matrix/Analyte: **Labs: Pass:** 13 **Fail:** 6 **Total:** 19

Potable Water trans-1,2-Dichloroethene

Shipment: 407 **Matrix:** Potable Water
Analyte: trans-1,2-Dichloroethene
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 2.66 ug/L
Limits: 1.6 to 3.72 ug/L
Basis: Fixed Percent (2)
Robust Mean: 2.9 ug/L
Std Dev: 0.5952 ug/L
Median: 2.865 ug/L

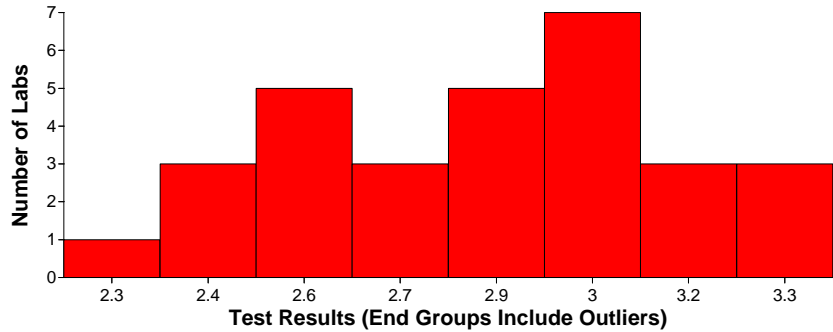

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 **Fail:** 1 **Total:** 30

Totals for Matrix/Analyte: **Labs: Pass:** 30 **Fail:** 1 **Total:** 31

Potable Water trans-1,2-Dichloroethene

Shipment: 407 **Matrix:** Potable Water
Analyte: trans-1,2-Dichloroethene
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 2.66 ug/L
Limits: 1.6 to 3.72 ug/L
Basis: Fixed Percent (2)
Robust Mean: 3.2 ug/L
Std Dev: 0 ug/L
Median: 3.18 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 **Fail:** 0 **Total:** 1

Totals for Matrix/Analyte: **Labs: Pass:** 30 **Fail:** 1 **Total:** 31

Potable Water tert-Butylbenzene

Shipment: 407 **Matrix:** Potable Water
Analyte: tert-Butylbenzene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 13.7 ug/L
Limits: 11 to 16.4 ug/L
Basis: Fixed Percent (2)
Robust Mean: 13.4 ug/L
Std Dev: 3.5819 ug/L
Median: 13.5 ug/L

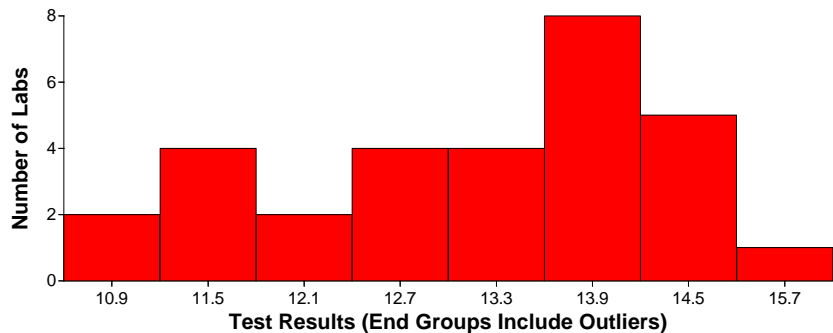

Totals for Matrix/Analyte/Technology:

Labs: Pass: 27 **Fail:** 3 **Total:** 30

Totals for Matrix/Analyte: **Labs: Pass:** 28 **Fail:** 3 **Total:** 31

Potable Water tert-Butylbenzene

Shipment: 407 Matrix: Potable Water
Analyte: tert-Butylbenzene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 13.7 ug/L
Limits: 11 to 16.4 ug/L
Basis: Fixed Percent (2)
Robust Mean: 12.1 ug/L
Std Dev: 0 ug/L
Median: 12.1 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 28 Fail: 3 Total: 31

Potable Water Trichloroacetic acid

Shipment: 407 Matrix: Potable Water
Analyte: Trichloroacetic acid
Sample: 0726
Technology: GC-ECD
Prep Method:
Target: 16.5 ug/L
Limits: 9.9 to 23.1 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 15.7 ug/L
Std Dev: 1.8092 ug/L
Median: 15.4 ug/L

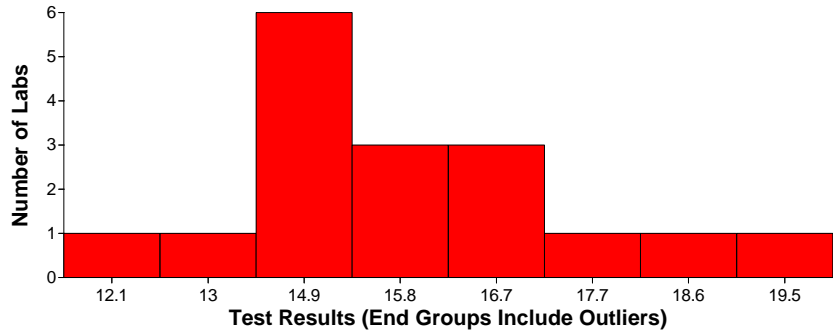

Totals for Matrix/Analyte/Technology:

Labs: Pass: 17 Fail: 0 Total: 17

Totals for Matrix/Analyte: Labs: Pass: 18 Fail: 0 Total: 18

Potable Water Trichloroacetic acid

Shipment: 407 Matrix: Potable Water
Analyte: Trichloroacetic acid
Sample: 0726
Technology: IC-ESI-MS
Prep Method:
Target: 16.5 ug/L
Limits: 9.9 to 23.1 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: ug/L
Std Dev: 0 ug/L
Median: 21.8 ug/L

A histogram is not displayed for Technology: IC-ESI-MS due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 18 Fail: 0 Total: 18

Potable Water Tetrachloroethene

Shipment: 407 Matrix: Potable Water
Analyte: Tetrachloroethene
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 5.64 ug/L
Limits: 3.38 to 7.9 ug/L
Basis: Fixed Percent (2)
Robust Mean: 5.5 ug/L
Std Dev: 1.2201 ug/L
Median: 5.48 ug/L

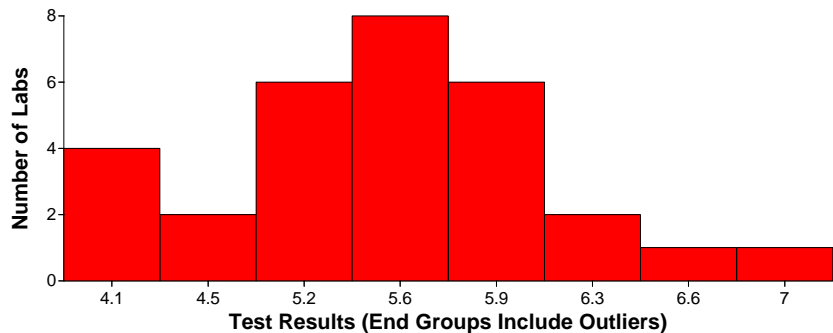

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water Tetrachloroethene

Shipment: 407 Matrix: Potable Water
 Analyte: Tetrachloroethene
 Sample: 0720
 Technology: GCELCD/PID
 Prep Method:
 Target: 5.64 ug/L
 Limits: 3.38 to 7.9 ug/L
 Basis: Fixed Percent (2)
 Robust Mean: 6.2 ug/L
 Std Dev: 0 ug/L
 Median: 6.23 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 1 Fail: 0 Total: 1
 Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

Potable Water Trifluralin


Shipment: 407 Matrix: Potable Water
 Analyte: Trifluralin
 Sample: 0707A
 Technology: GC-ECD
 Prep Method:
 Target: 7 ug/L
 Limits: 3.85 to 10.2 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 8.4 ug/L
 Std Dev: 0 ug/L
 Median: 8.44 ug/L

A histogram is not displayed for Technology: GC-ECD due to the limited number of participants.

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 1 Fail: 0 Total: 1
 Totals for Matrix/Analyte: Labs: Pass: 5 Fail: 1 Total: 6

Potable Water Trifluralin


Shipment: 407 Matrix: Potable Water
 Analyte: Trifluralin
 Sample: 0707A
 Technology: GC-MS
 Prep Method:
 Target: 7 ug/L
 Limits: 3.85 to 10.2 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 6.3 ug/L
 Std Dev: 2.4136 ug/L
 Median: 5.48 ug/L

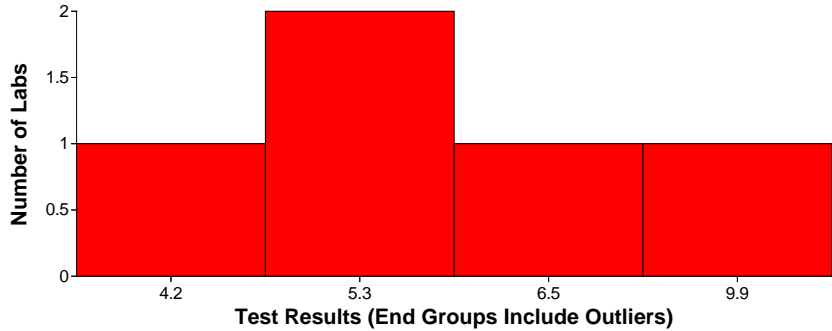

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 4 Fail: 1 Total: 5
 Totals for Matrix/Analyte: Labs: Pass: 5 Fail: 1 Total: 6

Potable Water Thallium, Total

Shipment: 407 Matrix: Potable Water
 Analyte: Thallium, Total
 Sample: 0706
 Technology: GFAAS
 Prep Method:
 Target: 7.5 ug/L
 Limits: 5.25 to 9.75 ug/L
 Basis: Target Value +/- a fixed percent
 Robust Mean: 7.5 ug/L
 Std Dev: 0.6245 ug/L
 Median: 7.37 ug/L

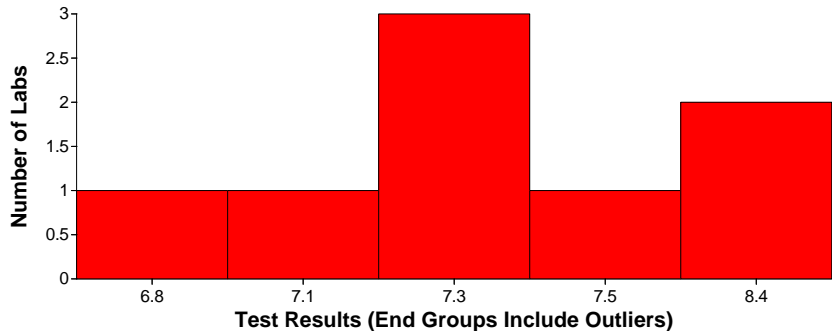

Totals for Matrix/Analyte/Technology:
 Labs: Pass: 8 Fail: 0 Total: 8
 Totals for Matrix/Analyte: Labs: Pass: 35 Fail: 1 Total: 36

Potable Water Thallium, Total


Potable Water Thallium, Total

Shipment: 407 Matrix: Potable Water
Analyte: Thallium, Total
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 7.5 ug/L
Limits: 5.25 to 9.75 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 7.5 ug/L
Std Dev: 2.387 ug/L
Median: 7.58 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 27 Fail: 1 Total: 28

Totals for Matrix/Analyte: Labs: Pass: 35 Fail: 1 Total: 36

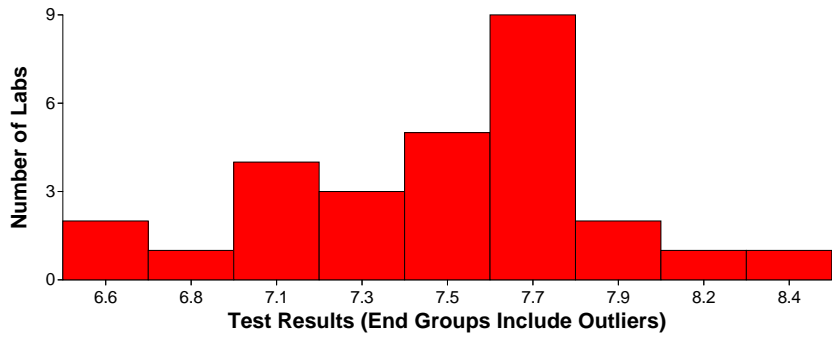


Potable Water Organic Carbon, Total

Shipment: 407 Matrix: Potable Water
Analyte: Organic Carbon, Total
Sample: 0733
Technology: IR
Prep Method:
Target: 2.79 mg/L
Limits: 2.23 to 3.35 mg/L
Basis: Target Value +/- a fixed percent
Robust Mean: 2.8 mg/L
Std Dev: 0.2868 mg/L
Median: 2.83 mg/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 17 Fail: 2 Total: 19

Totals for Matrix/Analyte: Labs: Pass: 17 Fail: 2 Total: 19

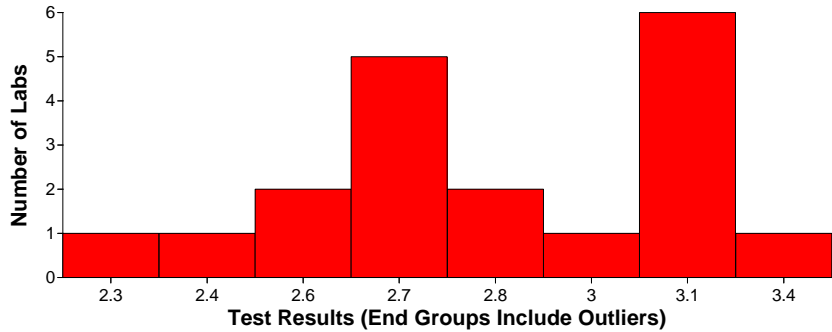


Potable Water Toluene

Shipment: 407 Matrix: Potable Water
Analyte: Toluene
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 7.55 ug/L
Limits: 4.53 to 10.6 ug/L
Basis: Fixed Percent (2)
Robust Mean: 7.4 ug/L
Std Dev: 1.4463 ug/L
Median: 7.4 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 29 Fail: 1 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

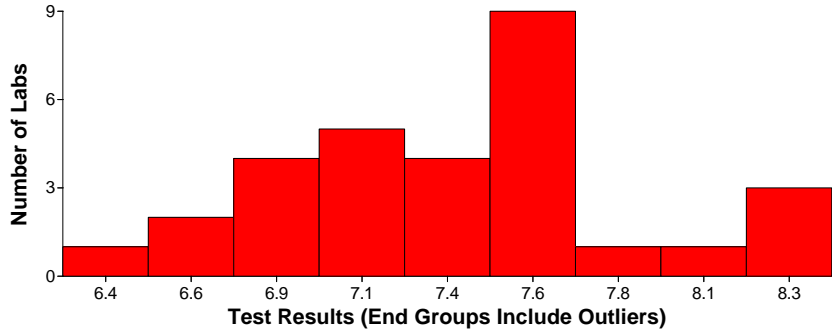

Potable Water Toluene

Shipment: 407 Matrix: Potable Water
Analyte: Toluene
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 7.55 ug/L
Limits: 4.53 to 10.6 ug/L
Basis: Fixed Percent (2)
Robust Mean: 6.8 ug/L
Std Dev: 0 ug/L
Median: 6.81 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1


Totals for Matrix/Analyte: Labs: Pass: 30 Fail: 1 Total: 31

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Potable Water Toxaphene

Potable Water Toxaphene

Shipment: 407 Matrix: Potable Water
Analyte: Toxaphene
Sample: 0716
Technology: GC-ECD
Prep Method:
Target: 9.18 ug/L
Limits: 5.05 to 13.3 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 9.8 ug/L
Std Dev: 1.3362 ug/L
Median: 10.08 ug/L

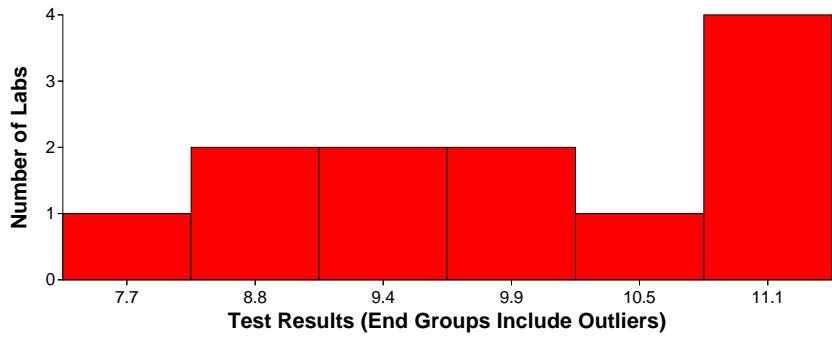

Totals for Matrix/Analyte/Technology:

Labs: Pass: 12 Fail: 0 Total: 12

Totals for Matrix/Analyte: Labs: Pass: 13 Fail: 0 Total: 13

Potable Water Toxaphene

Shipment: 407 Matrix: Potable Water
Analyte: Toxaphene
Sample: 0716
Technology: GC-MS
Prep Method:
Target: 9.18 ug/L
Limits: 5.05 to 13.3 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 8.8 ug/L
Std Dev: 0 ug/L
Median: 8.81 ug/L

A histogram is not displayed for Technology: GC-MS due to the limited number of participants.


Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 13 Fail: 0 Total: 13

Potable Water Trichloroethene

Shipment: 407 Matrix: Potable Water
Analyte: Trichloroethene
Sample: 0720
Technology: GC-MS
Prep Method:
Target: 10.9 ug/L
Limits: 8.72 to 13.1 ug/L
Basis: Fixed Percent (2)
Robust Mean: 11.2 ug/L
Std Dev: 2.9424 ug/L
Median: 11.05 ug/L

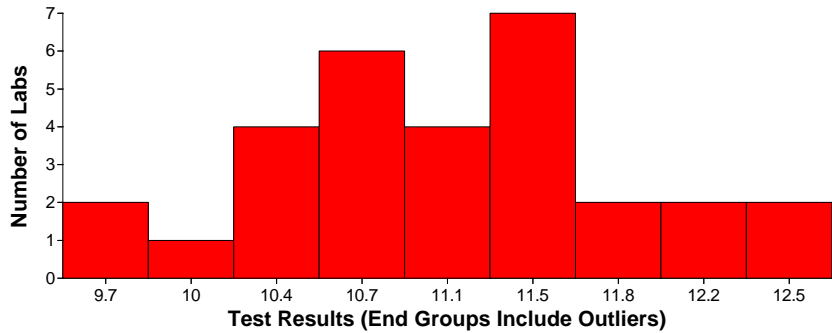

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 2 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water Trichloroethene

Shipment: 407 Matrix: Potable Water
Analyte: Trichloroethene
Sample: 0720
Technology: GCELCD/PID
Prep Method:
Target: 10.9 ug/L
Limits: 8.72 to 13.1 ug/L
Basis: Fixed Percent (2)
Robust Mean: 10.7 ug/L
Std Dev: 0 ug/L
Median: 10.7 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water Turbidity

Potable Water Turbidity

Shipment: 407 Matrix: Potable Water
Analyte: Turbidity
Sample: 0734
Technology: COLOR
Prep Method:
Target: 2.14 NTU
Limits: 1.77 to 2.52 NTU
Basis: Linear Regression
Robust Mean: 2.1 NTU
Std Dev: 0.5979 NTU
Median: 2.075 NTU

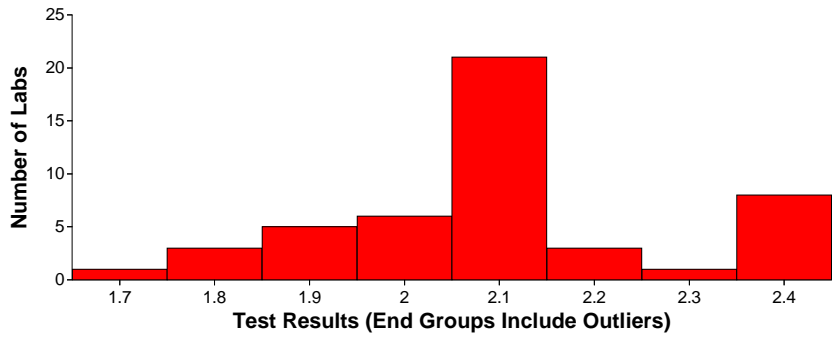


Totals for Matrix/Analyte/Technology:

Labs: Pass: 43 Fail: 5 Total: 48

Totals for Matrix/Analyte: Labs: Pass: 43 Fail: 5 Total: 48

Potable Water Total Xylenes

Shipment: 407 Matrix: Potable Water
Analyte: Total Xylenes
Sample: 0721
Technology: GC-MS
Prep Method:
Target: 32.3 ug/L
Limits: 25.8 to 38.8 ug/L
Basis: Fixed Percent (2)
Robust Mean: 32.2 ug/L
Std Dev: 8.4109 ug/L
Median: 32.35 ug/L

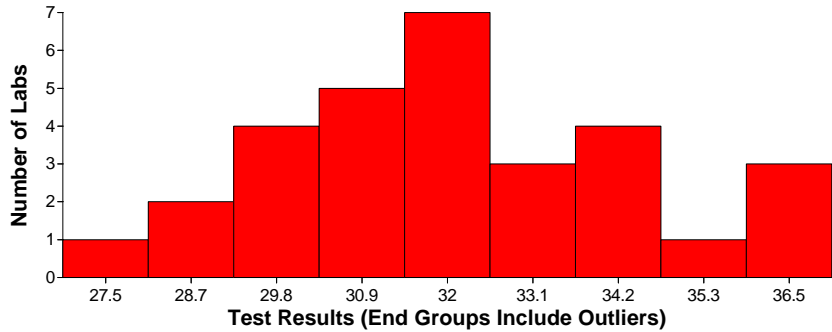

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 2 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water Total Xylenes

Shipment: 407 Matrix: Potable Water
Analyte: Total Xylenes
Sample: 0721
Technology: GCELCD/PID
Prep Method:
Target: 32.3 ug/L
Limits: 25.8 to 38.8 ug/L
Basis: Fixed Percent (2)
Robust Mean: 29.1 ug/L
Std Dev: 0 ug/L
Median: 29.1 ug/L

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

Potable Water Uranium (Mass)

Shipment: 407 Matrix: Potable Water
Analyte: Uranium (Mass)
Sample: 0706
Technology: COLOR
Prep Method:
Target: 80.1 ug/L
Limits: 65.3 to 88.2 ug/L
Basis: Linear Regression
Robust Mean: 81.2 ug/L
Std Dev: 0 ug/L
Median: 81.2 ug/L

A histogram is not displayed for Technology: COLOR due to the limited number of participants.

Totals for Matrix/Analyte/Technology:


Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 8 Fail: 0 Total: 8

Potable Water Uranium (Mass)

Potable Water Uranium (Mass)


Shipment: 407 **Matrix:** Potable Water
Analyte: Uranium (Mass)
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 80.1 ug/L
Limits: 65.3 to 88.2 ug/L
Basis: Linear Regression
Robust Mean: 77.9 ug/L
Std Dev: 3.5791 ug/L
Median: 79 ug/L

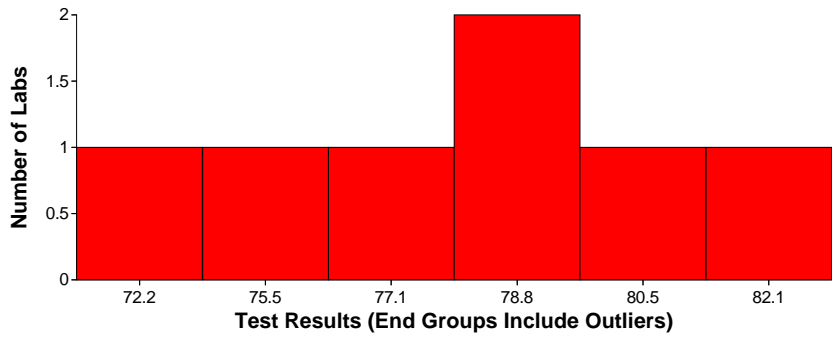

Totals for Matrix/Analyte/Technology:
Labs: Pass: 7 **Fail:** 0 **Total:** 7
Totals for Matrix/Analyte: **Labs: Pass:** 8 **Fail:** 0 **Total:** 8

Potable Water UV 254


Shipment: 407 **Matrix:** Potable Water
Analyte: UV 254
Sample: 0739
Technology: COLOR
Prep Method:
Target: 0.0821 cm -1
Limits: 0.0646 to 0.107 cm -1
Basis: Linear Regression
Robust Mean: 0.1 cm -1
Std Dev: 0.0122 cm -1
Median: 0.09 cm -1

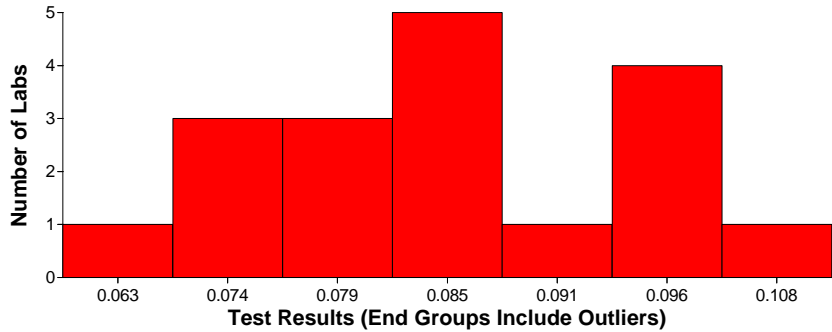

Totals for Matrix/Analyte/Technology:
Labs: Pass: 17 **Fail:** 1 **Total:** 18
Totals for Matrix/Analyte: **Labs: Pass:** 17 **Fail:** 1 **Total:** 18

Potable Water Vanadium, Total


Shipment: 407 **Matrix:** Potable Water
Analyte: Vanadium, Total
Sample: 0706
Technology: ICP-AES
Prep Method:
Target: 350 ug/L
Limits: 298 to 403 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 344.3 ug/L
Std Dev: 99.8722 ug/L
Median: 342 ug/L

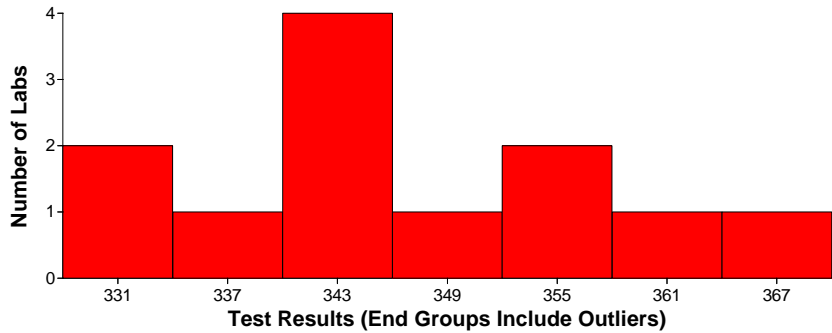

Totals for Matrix/Analyte/Technology:
Labs: Pass: 11 **Fail:** 1 **Total:** 12
Totals for Matrix/Analyte: **Labs: Pass:** 25 **Fail:** 1 **Total:** 26

Potable Water Vanadium, Total

Shipment: 407 **Matrix:** Potable Water
Analyte: Vanadium, Total
Sample: 0706
Technology: ICP-MS
Prep Method:
Target: 350 ug/L
Limits: 298 to 403 ug/L
Basis: Target Value +/- a fixed percent
Robust Mean: 342.9 ug/L
Std Dev: 13.5922 ug/L
Median: 342.5 ug/L

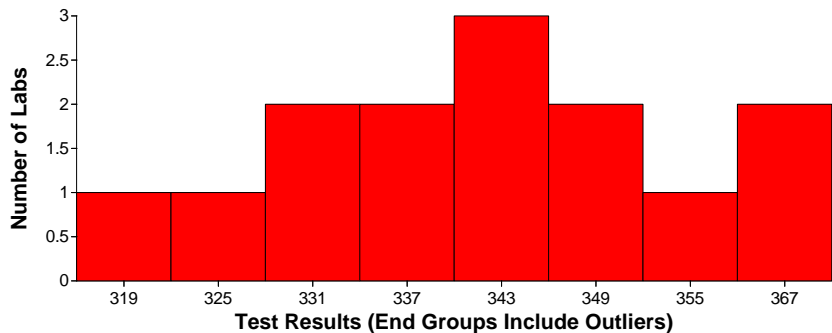

Totals for Matrix/Analyte/Technology:
Labs: Pass: 14 **Fail:** 0 **Total:** 14
Totals for Matrix/Analyte: **Labs: Pass:** 25 **Fail:** 1 **Total:** 26

Potable Water Vinyl chloride

Potable Water Vinyl chloride

Shipment: 407 Matrix: Potable Water

Analyte: Vinyl chloride

Sample: 0720

Technology: GC-MS

Prep Method:

Target: 9.9 ug/L

Limits: 5.94 to 13.9 ug/L

Basis: Target Value +/- a fixed percent

Robust Mean: 10.8 ug/L


Std Dev: 2.4444 ug/L

Median: 10.55 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 28 Fail: 2 Total: 30

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

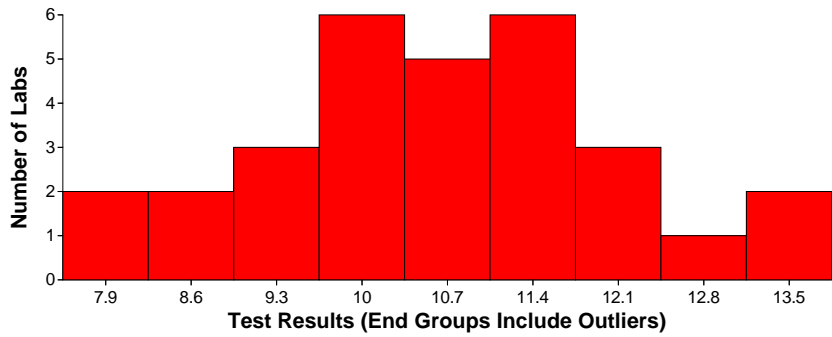

Potable Water Vinyl chloride

Shipment: 407 Matrix: Potable Water

Analyte: Vinyl chloride

Sample: 0720

Technology: GCELCD/PID

Prep Method:

Target: 9.9 ug/L

Limits: 5.94 to 13.9 ug/L

Basis: Target Value +/- a fixed percent

Robust Mean: 10.7 ug/L

Std Dev: 0 ug/L

Median: 10.7 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 1 Fail: 0 Total: 1

Totals for Matrix/Analyte: Labs: Pass: 29 Fail: 2 Total: 31

A histogram is not displayed for Technology: GCELCD/PID due to the limited number of participants.

Potable Water Oxamyl

Shipment: 407 Matrix: Potable Water

Analyte: Oxamyl

Sample: 0715

Technology: HPLC-FLUOR

Prep Method:

Target: 26.1 ug/L

Limits: 19.6 to 32.6 ug/L

Basis: Target Value +/- a fixed percent

Robust Mean: 25.8 ug/L


Std Dev: 1.7621 ug/L

Median: 25.6 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 9 Fail: 0 Total: 9

Totals for Matrix/Analyte: Labs: Pass: 9 Fail: 0 Total: 9

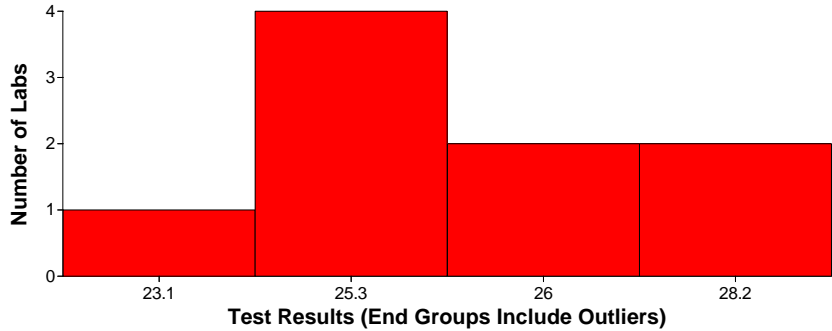

Potable Water Zinc, Total

Shipment: 407 Matrix: Potable Water

Analyte: Zinc, Total

Sample: 0706

Technology: FAAS

Prep Method:

Target: 550 ug/L

Limits: 468 to 633 ug/L

Basis: Target Value +/- a fixed percent

Robust Mean: 553 ug/L


Std Dev: 11.9583 ug/L

Median: 557 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 5 Fail: 0 Total: 5

Totals for Matrix/Analyte: Labs: Pass: 53 Fail: 4 Total: 57

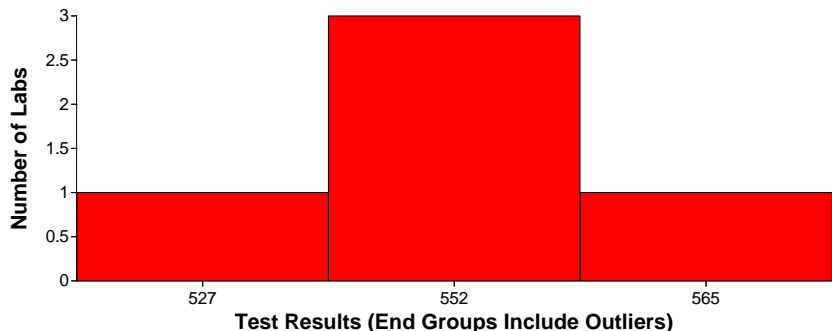

Potable Water Zinc, Total

Potable Water Zinc, Total

Shipment: 407 Matrix: Potable Water

Analyte: Zinc, Total

Sample: 0706

Technology: ICP-AES

Prep Method:

Target: 550 ug/L

Limits: 468 to 633 ug/L

Basis: Target Value +/- a fixed percent

Robust Mean: 548.9 ug/L


Std Dev: 151.051 ug/L

Median: 552.5 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 24 Fail: 2 Total: 26

Totals for Matrix/Analyte: Labs: Pass: 53 Fail: 4 Total: 57

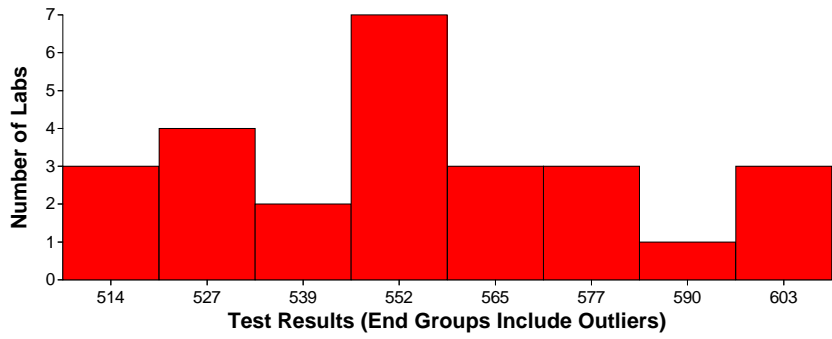

Potable Water Zinc, Total

Shipment: 407 Matrix: Potable Water

Analyte: Zinc, Total

Sample: 0706

Technology: ICP-MS

Prep Method:

Target: 550 ug/L

Limits: 468 to 633 ug/L

Basis: Target Value +/- a fixed percent

Robust Mean: 552.8 ug/L

Std Dev: 152.1162 ug/L

Median: 552 ug/L

Totals for Matrix/Analyte/Technology:

Labs: Pass: 24 Fail: 2 Total: 26

Totals for Matrix/Analyte: Labs: Pass: 53 Fail: 4 Total: 57

